

Supplementary Materials

Application of micro-tubing reeling system to serial femtosecond crystallography


Jihan Kim ^{1,#}, Sehan Park ^{2,#}, Yunje Cho ^{1,*} and Jaehyun Park ^{2,*}

¹Department of Life Sciences, Pohang University of Science and Technology, Pohang 37673, Republic of Korea

²Pohang Accelerator Laboratory, Pohang University of Science and Technology, Pohang 37673, Republic of Korea

*Correspondence: yunje@postech.ac.kr, jaehyun.park@postech.ac.kr

#Equally contributed to this work

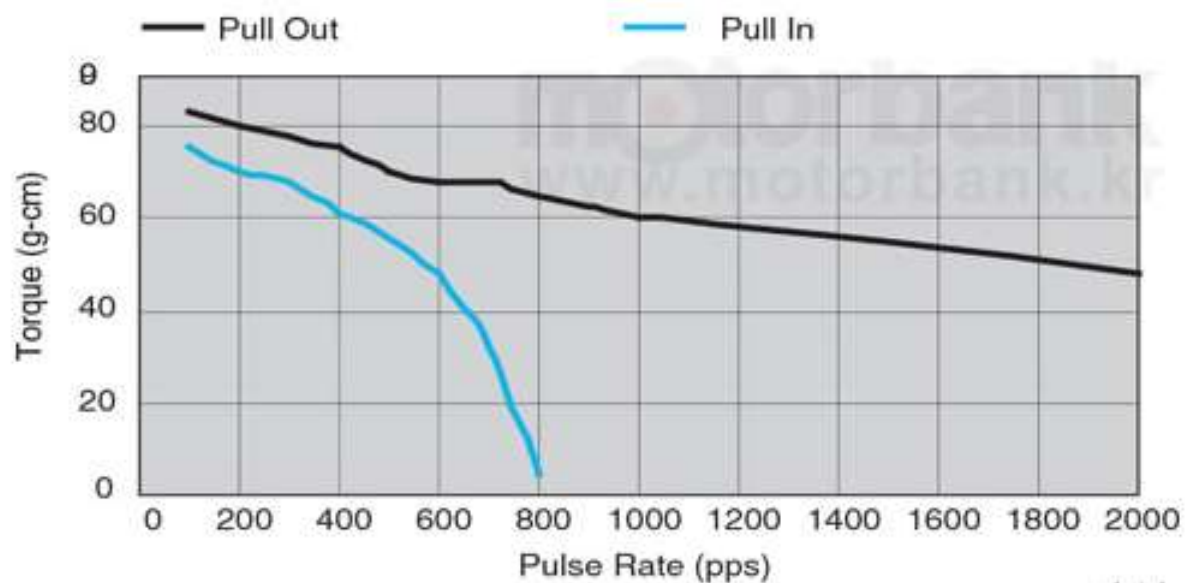

Supplementary Fig. 1 Relation between pps and torque of the mini-rotor. The torque value was estimated from the curve of “Pull In”.

Supplementary Mov. 1 Real-time view of the MRS operation during the SFX experiment. The MCC is moving from right to left direction during the operation. This monitoring movie was taken with a long working distance microscope (WD=300mm) installed at the MICOSS.