
Article

Not peer-reviewed version

Characterization of hFOB 1.19 Cell Line for Studying Zn-Based Degradable Metallic Biomaterials

[Eva Jablonská](#) ^{*}, [Lucie Mrázková](#), [Jiří Kubásek](#), [Dalibor Vojtěch](#), [Irena Paulin](#), [Tomáš Ruml](#), [Jan Lipov](#)

Posted Date: 30 January 2024

doi: [10.20944/preprints202401.2053.v1](https://doi.org/10.20944/preprints202401.2053.v1)

Keywords: zinc degradable materials, in vitro cytotoxicity testing, hFOB 1.19 osteoblasts



Preprints.org is a free multidiscipline platform providing preprint service that is dedicated to making early versions of research outputs permanently available and citable. Preprints posted at Preprints.org appear in Web of Science, Crossref, Google Scholar, Scilit, Europe PMC.

Copyright: This is an open access article distributed under the Creative Commons Attribution License which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Disclaimer/Publisher's Note: The statements, opinions, and data contained in all publications are solely those of the individual author(s) and contributor(s) and not of MDPI and/or the editor(s). MDPI and/or the editor(s) disclaim responsibility for any injury to people or property resulting from any ideas, methods, instructions, or products referred to in the content.

Article

Characterization of hFOB 1.19 Cell Line for Studying Zn-Based Degradable Metallic Biomaterials

Eva Jablonská ^{1,*}, Lucie Mrázková ¹, Jiří Kubásek ², Dalibor Vojtěch ², Irena Paulin ³, Tomáš Ruml ¹ and Jan Lipov ¹

¹ Department of Biochemistry and Microbiology, University of Chemistry and Technology, Prague, Technická 5, 166 28 Prague 6, Czech Republic

² Department of Metals and Corrosion Engineering, University of Chemistry and Technology, Prague, Technická 5, 166 28 Prague 6, Czech Republic

³ Department Physics and Chemistry of Materials, Institute of Metals and Technology, University of Ljubljana, Lepi pot 11, SI-1000 Ljubljana, Slovenia

* Correspondence: eva.jablonska@vscht.cz

Abstract: In vitro testing is the first important step in the development of new biomaterials. The human fetal osteoblast cell line hFOB 1.19 is a very promising cell model; however, there are vast discrepancies in cultivation protocols, especially in the cultivation temperature and the presence of selection reagent, genetin (G418). We intended to use hFOB 1.19 for the testing of Zn-based degradable metallic materials. However, the sensitivity of hFOB 1.19 to zinc ions has not yet been studied. Therefore, we compared the toxicity of zinc towards hFOB 1.19 under different conditions and compared it with that of the L929 mouse fibroblast cell line. We also tested the cytotoxicity of three types of Zn-based biomaterials in two types of media. The presence of G418 used as a selection reagent decreased the sensitivity of hFOB 1.19 to Zn²⁺. hFOB 1.19 were more sensitive to Zn²⁺ at elevated (restrictive) temperatures. hFOB 1.19 were less sensitive to Zn²⁺ than L929 (both as ZnCl₂ and extracts of alloys). Therefore, the appropriate cultivation conditions of hFOB 1.19 during biomaterial testing should be chosen with caution.

Keywords: zinc degradable materials; in vitro cytotoxicity testing; hFOB 1.19 osteoblasts

1. Introduction

The first important step in the development of any biomaterial is in vitro cytotoxicity testing, although it cannot encompass all of the complexities in the body. In addition to biomaterials intended for permanent bone implants, there is also an increasing interest in degradable metallic biomaterials for temporary bone fixation (reviewed in [1]). Here, we focus on zinc-based biomaterials for orthopedic applications, which have been the subject of interest in the last decade [2–5]. The corrosion rate and toxicity of in vitro tests often do not correlate with those *in vivo*. (e.g., [5–7]). There are probably many reasons for this (e.g., lack of circulation of body fluids, only one cell type used, 2D cell arrangement in vitro [8–10]), nevertheless, the appropriate cell model can also play a prominent role [11].

There are two main options for choosing the in vitro model: primary cells or cancer-derived cell lines. The former reliably mimics properties of the tissue *in vivo*; however, the cells have a limited lifespan and a high variability within donors, which hinders their routine use in experiments. Continuous cell lines represent an unlimited cell source for testing, since they can proliferate indefinitely. However, their behavior differs significantly from that of primary cells, and thus of the cells in tissues. A compromise choice may be cells obtained by so-called gentle cell immortalization, for example, their transfection with a gene coding a temperature-sensitive mutant of SV40 large T antigen (tsA58), since it can lead to a combination of advantageous properties of both types mentioned above. At a lower (permissive) temperature, tsA58 is active and promotes cell proliferation. At elevated (restrictive) temperature, cells stop dividing and can differentiate into mature cell types [12,13].

The ISO 10993-5 standard [14] mentions the L929 murine fibroblast cell line (ATCC CCL-1) as a possible cell model to be used in in vitro biomaterial testing. Specifically, for the cytocompatibility testing of biomaterials intended for orthopedic applications, osteoblast-like cancer cell lines (e.g., U-2 OS, MG-63, and Saos-2) are used; however, none of them can be considered a reliable substitute for human osteoblasts [15,16].

To date, the biological response of newly prepared Zn alloys has been performed on cell cultures of various origins (reviewed, e.g., in [17]), mainly on L929 and on osteoblast-like cell lines MG-63 and MC3T3-E1 [18]. However, there is a demand to use the appropriate and preferably non-cancerous cell line for the intended application for cytotoxicity evaluation [11]. We have previously shown that the cancerous osteoblast-like cell line U-2 OS is less sensitive than the L929 cell line to zinc ions [19]. Here, we present the conditionally immortalized human fetal osteoblast cell line hFOB 1.19 (ATCC CRL-11372), established by Harris et al. (1995), as a suitable model for degradable zinc-based biomaterials, as it is not cancerous and has the characteristics of osteoblasts.

The cell line hFOB 1.19 was derived from biopsies of limb tissue from a spontaneous miscarriage and immortalized by transfection with tsA58. The selection reagent G418 (geneticin) facilitated the initial selection of transfected cells and, at a reduced concentration ($300 \mu\text{g}\cdot\text{ml}^{-1}$), it ensures further maintenance of the transgene cells during long-term cultivation [20].

The cell line hFOB 1.19 was further characterized by Subramaniam et al. who showed that this cell line was capable of bone formation in vivo and the analysis of the karyotype showed only minimal chromosomal changes [21]. Furthermore, Yen et al. observed the multilineal differentiation potential (toward adipocytes or chondrocytes) of hFOB 1.19 cells under appropriate conditions [22]. Marozin et al. even claimed that hFOB 1.19 can serve as a surrogate model for bone marrow-derived mesenchymal stromal cells [23].

However, there are also great discrepancies in the cultivation protocols. There is disagreement on the interpretation of the restrictive temperature. ATCC, the cell supplier, states 39.5°C in their protocols, but some authors choose 37°C for their experiments for culture differentiation [24–27]. On the contrary, some authors consider 37°C to be a permissive temperature [28,29]. It is also not clear whether the G418 selection reagent should be added during osteodifferentiation.

The hFOB 1.19 cell line has already been used in cancer research and osteomyelitis research [25,30] as well as in studies with permanent [31,32], and degradable [24,33] biomaterials. There are also studies that use hFOB 1.19 for testing of degradable materials doped with Zn (Table 1). However, the sensitivity of the hFOB 1.19 cell line to Zn^{2+} has not yet been studied.

Here, we compare the sensitivity of L929 and hFOB 1.19 cell lines to Zn^{2+} in different media, as well as the effect of temperature on the metabolic activity of hFOB 1.19 and on its sensitivity to Zn^{2+} .

Table 1. Studies using hFOB 1.19 for the testing of degradable biomaterials containing Zn (HA = hydroxyapatite).

Material	G418	Temperatures	Reference
sol-gel-prepared glass materials with ZnO	not mentioned	37°C as permissive 39.5°C as restrictive	[29]
Zn-doped HA coatings	not mentioned	37°C	[34]
Reactive interfaces based on hydroxides-	present	37°C	[35]
Zn rich HA			
3D porous granules based on Zn-containing CaPs	present	34°C	[36]
Zn- doped HA nanopowders	not mentioned	34°C	[37].

HA and bimetallic nanocomposite of ZnO-Ag	present	34 °C	[38]
Zn-doped nanoHA-based bone scaffolds	present	34 °C	[39]

2. Materials and Methods

2.1. Cell cultivation

hFOB 1.19 (ATCC CRL-1137) were maintained in DMEM/Ham's F-12 medium without phenol red (Sigma, D6434) supplemented with 10% FBS (Sigma, F7524), 2.5mM L-glutamine (Sigma, G7513) and selection reagent G418 (Sigma, G8168) at a final concentration of 0.3 mg·ml⁻¹ at 34 °C, 5% CO₂ and 100% relative humidity. Cells were passaged regularly when sub-confluent using a trypsin-EDTA solution without phenol red (Gibco, 15400054).

Murine fibroblasts L929 (ATCC CCL-1) were maintained in MEM (Sigma, M0446) medium supplemented with 10% FBS (FBS, Sigma F7524) under standard conditions of 37 °C, 5% CO₂ and 100% relative humidity. Cells were passaged regularly when sub-confluent using trypsin-EDTA solution (Sigma, T4049).

2.2. Preparation of the ZnCl₂ solution

The 10mM stock solution of ZnCl₂ was prepared in dH₂O and sterilized by filtration. Fresh working solutions (from 40µM up to 360µM) were prepared in cultivation medium prior to the experiment.

2.3. Preparation of the materials

In the present study, three different materials, which were considered promising for future applications in the development of medical devices (Table 2), were used for cytotoxicity tests. Details of the procedure are given in [40–43].

Cylindrical samples (5 mm in diameter and 2 mm in height) were ground (SiC paper, with the grit size up to P4000), cleaned, and sterilized by immersion in 70% ethanol (2 h) and by subsequent exposure to UV (2 h).

Table 2. Materials used for testing.

Designation (composition in wt. %)	Synthesis	Processing conditions (temperature and extrusion ratio)
Zn-1Mg	Powder metallurgy	Extrusion of powder billets at 200 °C and extrusion ratio 25
Zn-1Mg-1Ag	Powder metallurgy	Extrusion of powder billets at 200 °C and extrusion ratio 25
Zn-0.8Mg-0.2Ag	Conventional casting and extrusion	Extrusion of casted ingot at 200 °C and extrusion ratio 25

2.4. Preparation of the extracts

The prepared samples were transferred to MEM or DMEM/Ham's F-12 cultivation medium with 5% fetal bovine serum (FBS) and agitated (130 RPM) at 37 °C in closed vessels for 24 hours. The surface to volume ratio was 87.5 cm²·ml⁻¹ for all samples. Four replicates were used for each sample for each medium. The extracts from four samples were then pooled. The extracts were used for

indirect *in vitro* cytotoxicity tests (undiluted, i.e., 100%, and diluted, i.e., 50% extracts were used) and for ICP-MS measurement.

2.5. Metabolic activity of hFOB 1.19 and cytotoxicity of Zn²⁺ towards hFOB 1.19 after long-term cultivation at different temperatures

hFOB 1.19 cells were seeded in 48-well plates in DMEM/Ham's F-12 medium without phenol red, with 10% FBS and with or without selection reagent G418. 48-well plates were used to facilitate medium exchanges. The seeding density was 263,000 cells·cm⁻². Cells were cultivated at 34 °C for 3 days until full confluence was reached. Subsequently, the cultivation continued at different temperatures (34, 37 or 39.5 °C). The medium was exchanged every 4-5 days. After 14 days of cultivation, the medium was exchanged for solutions of ZnCl₂ in medium with 5% FBS. After 24 h, metabolic activity was evaluated using the resazurin assay.

2.6. Cytotoxicity of Zn²⁺ and extracts towards hFOB 1.19 and L929 in different media

hFOB 1.19 or L929 cells were seeded in 96-well plates (20,000 cells/well in 50 µl, i.e., approx. 60,000 cells·cm⁻²) in DMEM/Ham's F-12 or in MEM medium with 10% FBS and cultivated for 4 hours at 34 °C or 37 °C, respectively. Subsequently, ZnCl₂ solutions in media without FBS (50 µl) were added to the cells to achieve the 5% FBS concentration. After one day, metabolic activity was evaluated using the resazurin assay.

2.7. Zn²⁺ and extracts cytotoxicity towards hFOB 1.19 and L929 in different media

hFOB 1.19 or L929 cells were seeded in 96-well plates (20,000 cells/well in 100 µl, i.e., approx. 60,000 cells·cm⁻²) in DMEM/Ham's F-12 or in MEM medium with 10% FBS and cultivated for 4 hours at 34 °C or 37 °C, respectively. Subsequently, the medium was replaced with alloy extracts in medium with 5% FBS (100 µl). After one day, metabolic activity was evaluated using the resazurin assay.

2.8. Evaluation of metabolic activity (resazurin assay)

Cell metabolic activity was evaluated using the resazurin assay [44]. Resazurin is metabolized to resorufin by living cells. Cell medium was aspirated and a resazurin solution (final concentration 25 µg·ml⁻¹) in medium without phenol red was added. After 1 h of incubation, fluorescence was measured at 560/590 nm (excitation/emission) (Fluoroskan Ascent FL, Thermo, or Spectramax id5, Molecular Devices). Metabolic activity was depicted as absolute fluorescence of resorufin. The cytotoxicity of the solutions and extracts was depicted as a percentage of the metabolic activity of the control (sole medium without zinc). Extracts that caused a decrease below 70 % of the activity of the control were considered cytotoxic, as described in the ISO 10993-5 standard.

2.9. ICP-MS measurement

The extracts were analyzed by inductively coupled plasma mass spectrometry (ICP-MS) using a Perkin Elmer Elan 6000 spectrometer (three measurements for each sample). Prior to the measurement, ultrapure HNO₃ was added to the extracts in order to dissolve the majority of solid corrosion products.

3. Results

Our main goal was to determine the sensitivity of hFOB 1.19 cells to Zn²⁺ at both permissive and restrictive temperatures. Due to the discrepancies in the published cultivation protocols, we used a temperature of 34 °C as proliferative and both temperatures of 37 °C and 39.5 °C as restrictive. We also used the medium with and without G418 selection reagent. The effect of zinc ions on cells under different conditions was then evaluated. We compared the results obtained for hFOB 1.19 with those of the L929 cell line, which is recommended for cytotoxicity tests according to the ISO-10993 standard.

We also used Zn-based biomaterials and performed a test with the extract according to ISO 10993-5 using both cell types.

The influence of selection reagent on the metabolic activity of hFOB 1.19

We compared the metabolic activity of cells after 7 and 14 days of incubation at different temperatures with and without the G418 selection reagent (Figure 1). After 7 days, metabolic activity was significantly lower in the absence of G418 at both restrictive temperatures compared to the permissive one. After 14 days, the difference between the variants with and without G418 was less profound and, surprisingly, was statistically significant both at the restrictive temperature and the permissive temperatures of 39.5 °C and 34 °C, respectively.

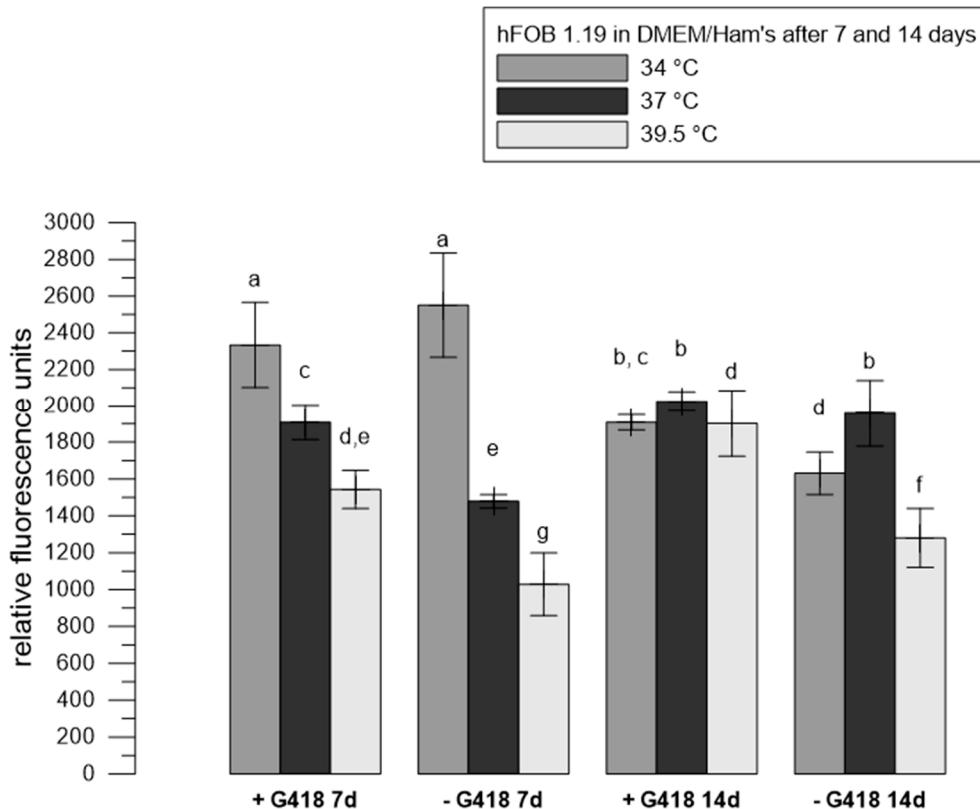


Figure 1. Resorufin fluorescence produced by hFOB 1.19 cells after 7 and 14 days of cultivation in the presence (+) and absence (-) of the G418 selection agent. The error bars indicate the sample standard deviation of three measurements (three wells). Differences ($p < 0.05$) among groups are indicated by letters (one-way ANOVA followed by Tukey test).

Zn^{2+} were more toxic to hFOB 1.19 cells at restrictive temperatures than at permissive temperatures

Figure 2 shows the metabolic activity (resazurin assay) of hFOB 1.19 cells after their one-day exposure to $ZnCl_2$ solutions preceded by 14-day incubation at different temperatures. No toxic effect of zinc ions was observed in cells cultured at 34 °C, even at the highest concentration of Zn^{2+} used (140 $\mu\text{mol}\cdot\text{l}^{-1}$). Cells cultured in the absence of G418 at restrictive temperatures were more sensitive to $ZnCl_2$ compared to those cultured in the presence of G418. The decrease below the normative cut-off was observed at a concentration of 140 $\mu\text{mol}\cdot\text{l}^{-1}$.

The possibility of G418 influencing the metabolic activity assay was excluded, because the medium with G418 was removed prior to the addition of $ZnCl_2$ solutions.

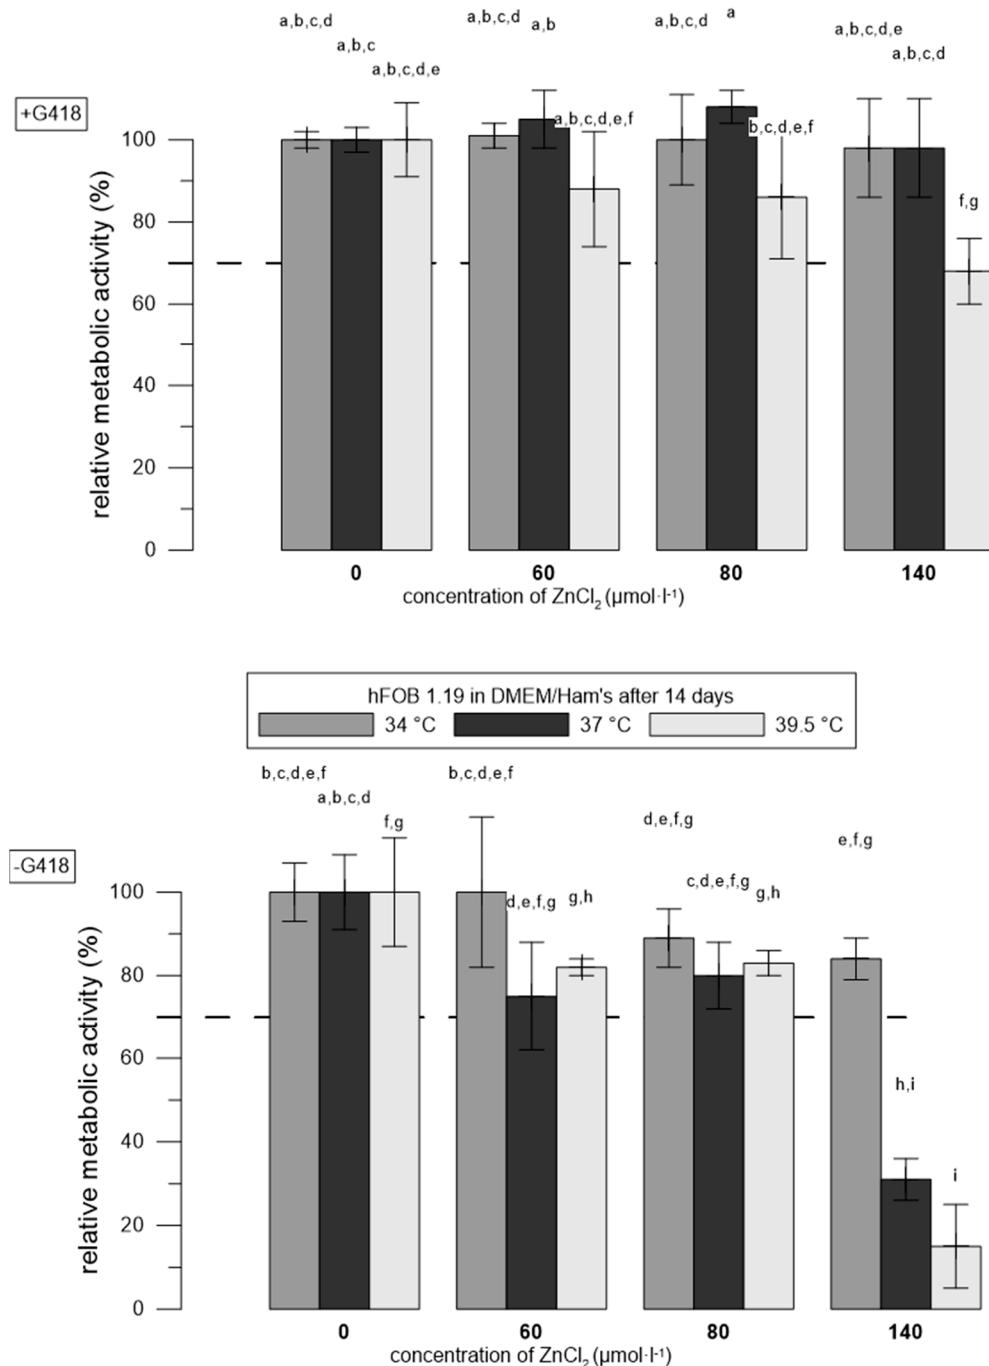


Figure 2. Relative metabolic activity of hFOB 1.19 cells after 14 days of differentiation in the presence (+) and absence (-) of the selection agent G418 after 1 day of incubation with ZnCl₂ solutions. Metabolic activity is expressed as a percentage (the negative control of 0 μmol·l⁻¹ ZnCl₂ represents 100%). Error bars indicate the sample standard deviation of three measurements (three wells). Differences (p < 0.05) among groups calculated from fluorescence values are indicated by letters (one-way ANOVA followed by Tukey test).

Zn²⁺ were more toxic to L929 than to hFOB 1.19 in the media recommended for each cell line

To compare the toxic effect of Zn²⁺ on L929 and hFOB 1.19, the same numbers of cells were seeded and after 4 h of incubation, the ZnCl₂ solutions were added.

Figure 3 shows that the mouse fibroblast cell line L929 was more sensitive to Zn²⁺ than hFOB 1.19 cells (a decrease in metabolic activity below 70 % was observed at 60 μmol·l⁻¹ concentration of ZnCl₂, while a toxic effect towards hFOB 1.19 cells was observed at 100 μmol·l⁻¹ ZnCl₂).

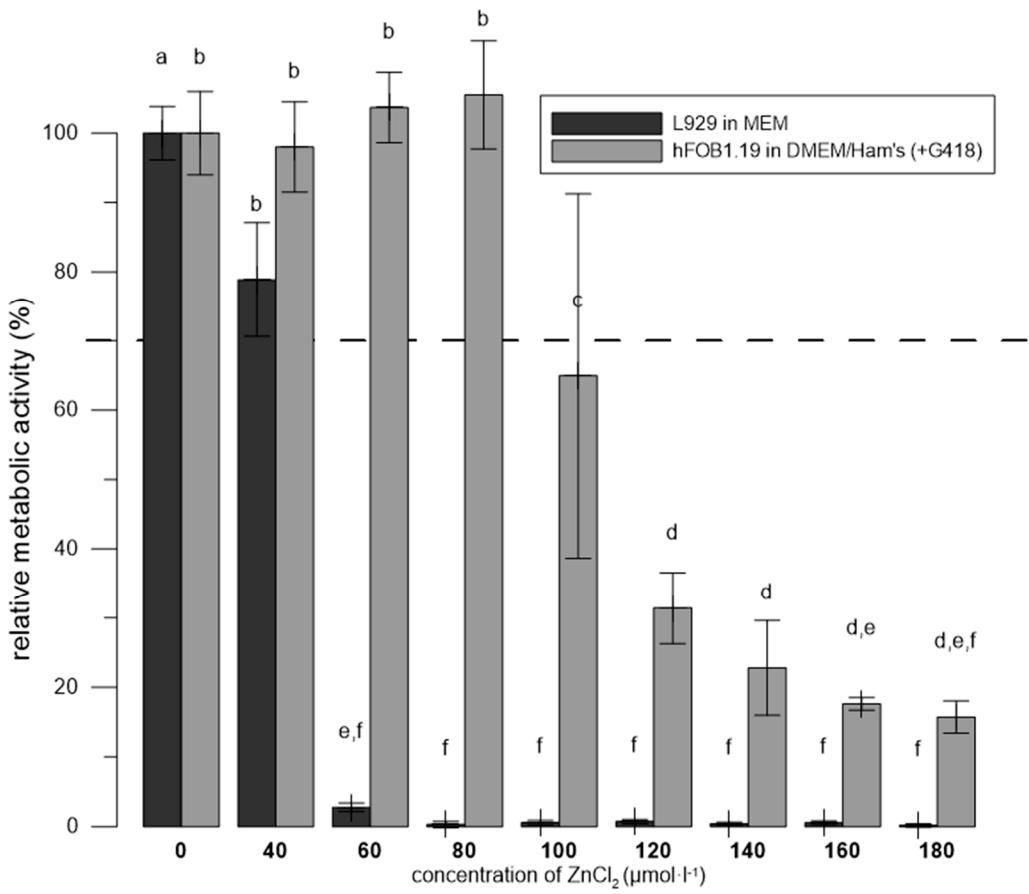


Figure 3. Relative metabolic activity of hFOB 1.19 and L929 cells after 1 day of incubation with ZnCl_2 solutions. Metabolic activity is expressed as a percentage (negative control lacking ZnCl_2 represents 100%). The error bars indicate the sample standard deviation of six measurements (six wells). Differences ($p < 0.05$) among groups calculated from fluorescence values are indicated by letters (One-way ANOVA followed by Tukey test).

The effect of media used

Different cultivation media for the cell lines were used in the previous experiment according to the recommendation of the manufacturer's. To evaluate the effect of the cultivation medium on the toxicity of Zn^{2+} , a test was performed with both MEM and DMEM/Ham's F-12 culture medium used for both hFOB 1.19 and L929 cell lines. Again, ZnCl_2 solutions were added 4 h after seeding the same number of both cell lines. We did not use G418 in this experiment to ensure the same conditions for both cell lines.

As in the previous experiment (Figure 3), the higher sensitivity of L929 compared to hFOB 1.19 cells was shown and the toxic effect at the $60\mu\text{mol}\cdot\text{l}^{-1}$ concentration of Zn^{2+} was also confirmed for the L929 cell line (Figure 4). Higher metabolic activity of L929 cells was observed in the MEM medium, which is recommended for this cell line. On the contrary, hFOB 1.19 cells withstood higher concentrations of ZnCl_2 in the DMEM/Ham's F-12 medium which is recommended for this cell line. The threshold toxic concentration of ZnCl_2 in the case of hFOB 1.19 cells in MEM was around $100\mu\text{mol}\cdot\text{l}^{-1}$.

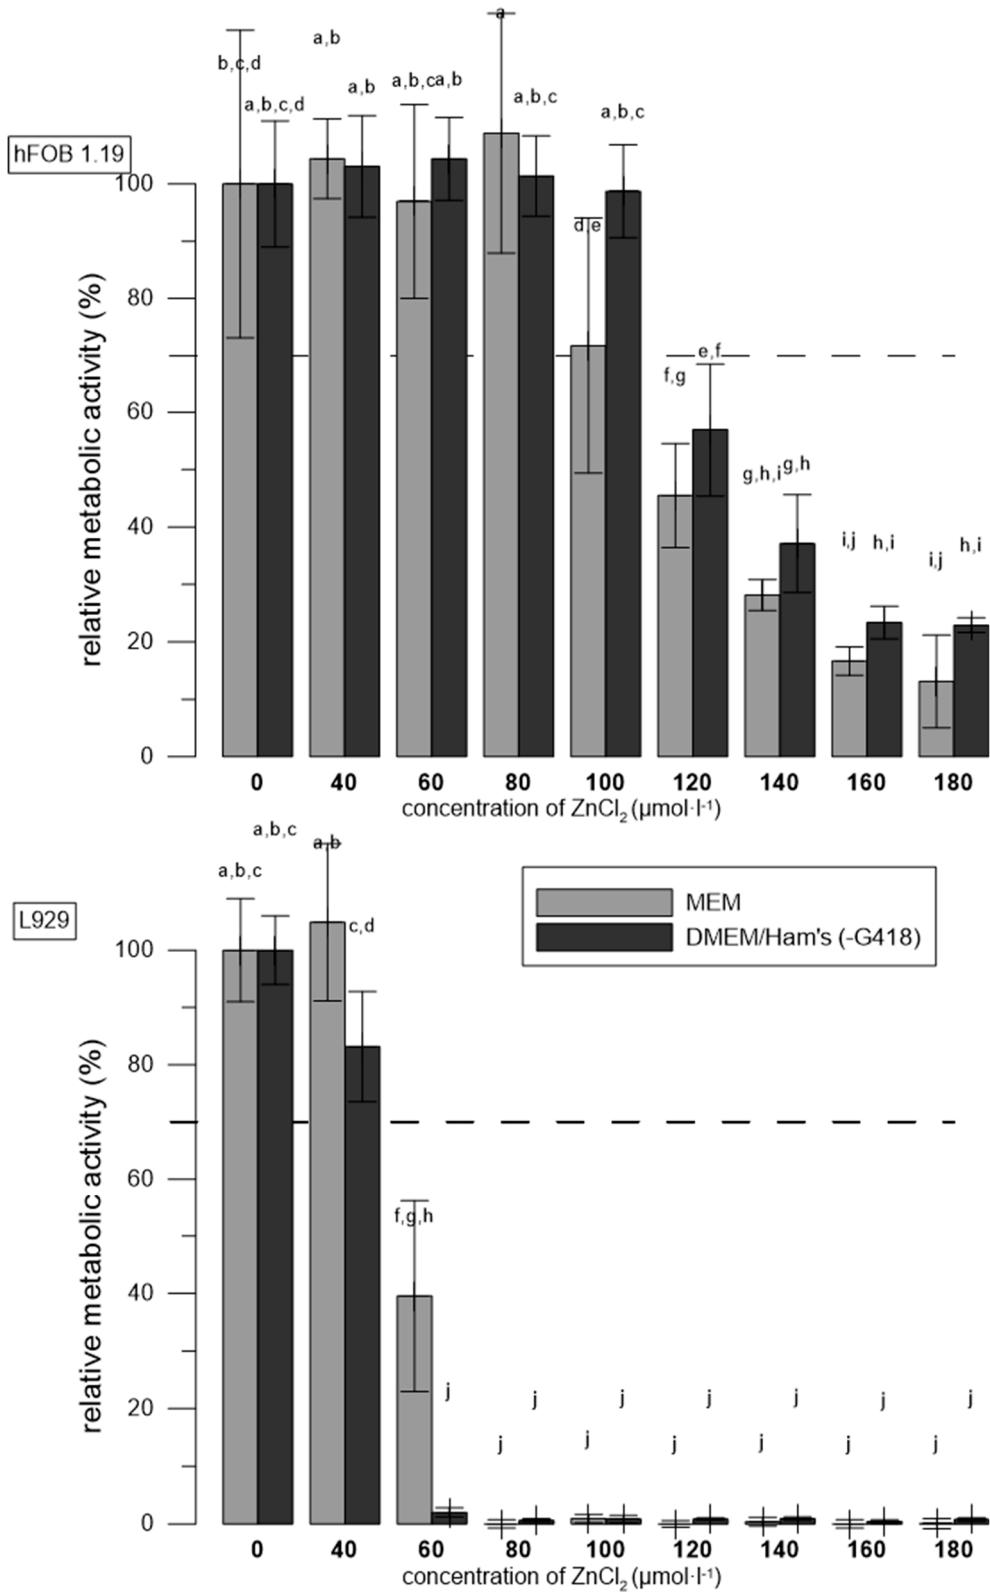


Figure 4. Relative metabolic activity of hFOB 1.19 and L929 cells after 1 day of incubation with ZnCl_2 solutions. Metabolic activity is expressed as percent (negative control without ZnCl_2 represents 100%). Error bars indicate the sample standard deviation of six measurements (six wells). Differences ($p < 0.05$) among groups are indicated by letters (one-way ANOVA followed by Tukey test).


Comparison of the cytotoxicity of extracts of alloys in different media towards hFOB 1.19 and L929

We also tested extracts of selected Zn-based degradable biomaterials according to ISO 10993-5. The extracts were prepared as described in section 2.4. The undiluted extracts of the alloys were toxic to both tested cell lines and almost completely inhibited the metabolic activity of both cell lines (relative metabolic activity was 7 % or less, data not shown). Therefore, only results with 50% extracts are presented. The Zn and Ag concentrations in the extracts were measured using ICP-MS. The concentration of Ag in the diluted extracts was below 1.8 nmol·l⁻¹ and was considered to have a minor effect. The concentration of Zn ranging between 72 and 102 µmol·l⁻¹ is shown for particular alloys on the labels above the columns of the graph. We did not observe any increase in pH after extraction using phenol red in cultivation medium as an indicator. This is in accordance with our previous studies [40].

Figure 5 shows that the extracts were more toxic to the L929 cell line. For example, the same extract of Zn-1Mg in DMEM/Ham's F-12 medium (Zn concentration = 73 µmol·l⁻¹) did not have any adverse effect on the hFOB 1.19 cell line; however, the metabolic activity of L929 was decreased to 2 %.

Generally, the extracts prepared in MEM were more toxic for the hFOB 1.19 cell line compared to the extract prepared in DMEM/Ham's F-12, even when they contained less Zn. For example, Zn-1Mg-1Ag extracts in DMEM/Ham's F-12 medium (Zn concentration = 90 µmol·l⁻¹) did not decrease the metabolic activity of hFOB 1.19 cells, while the Zn-1Mg-1Ag extract in MEM (Zn concentration = 72 µmol·l⁻¹), decreased the metabolic activity of hFOB 1.19 cells below 20 %.

The metabolic activity of L929 after exposition to all of the extract was 2 % or less. Therefore, the difference in toxicity of the extract in MEM and DMEM/Ham's F-12 is less evident.

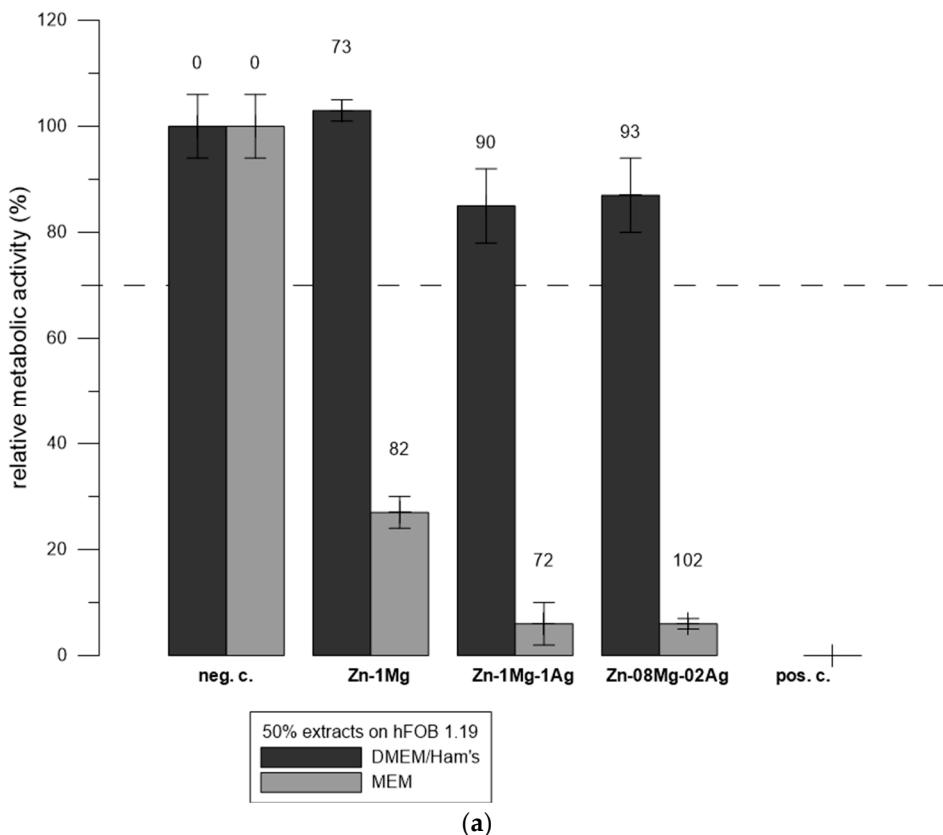

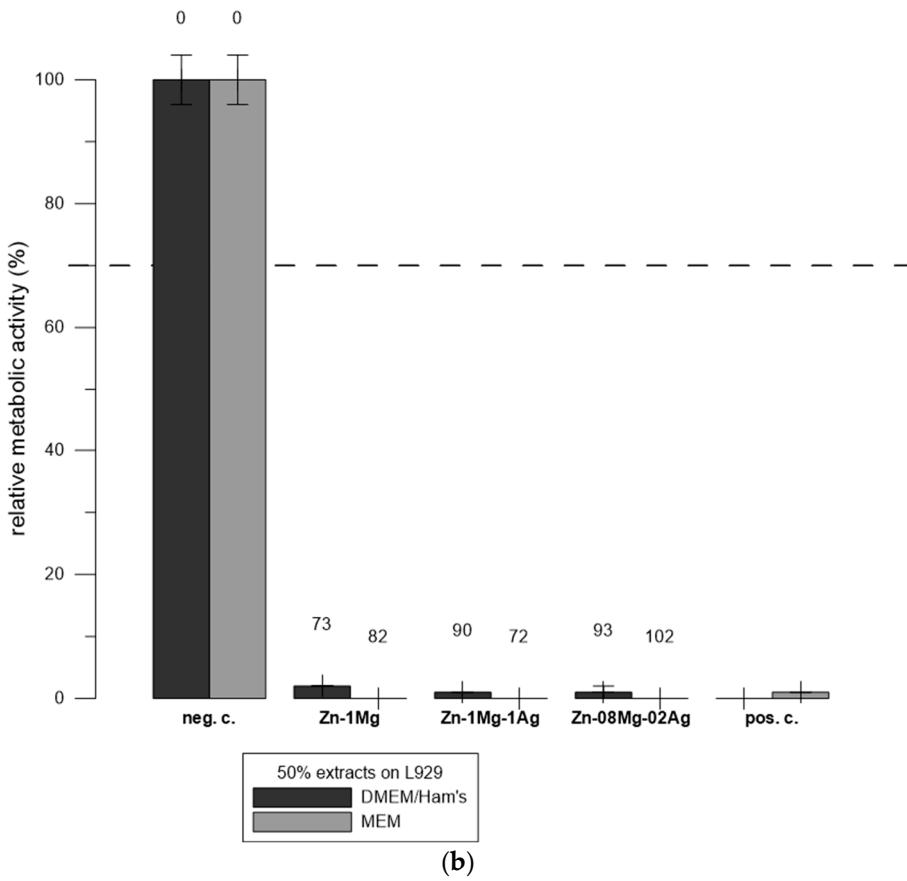


Figure 5. Relative metabolic activity of hFOB 1.19 (a) and L929 (b) cells after 1 day of incubation with extracts of Zn-based materials. Metabolic activity is expressed as a percentage (negative control of sole medium-represents 100%). Error bars indicate the sample standard deviation of six measurements (six wells). The labels above the columns indicate the concentration of Zn in $\mu\text{mol}\cdot\text{l}^{-1}$ measured by ICP-MS.

4. Discussion

Authors should discuss the results and how they can be interpreted from the perspective of previous studies and of the working hypotheses. The findings and their implications should be discussed in the broadest context possible. Future research directions may also be highlighted.

The human fetal osteoblast cell line hFOB 1.19 is a promising model for the in vitro testing of biomaterials due to its similarity to primary osteoblasts and its unlimited supply caused by conditional immortalization. However, the discrepancies in the cultivation protocols raise the question of what conditions should be chosen during the biomaterial tests.

First, we compared the sensitivity of hFOB 1.19 to Zn^{2+} in the presence and absence of the selection reagent G418. When establishing this cell line by Harris et al [20], G418 was used for the selection of transfectant and for additional maintenance during cultivation, since the desirable phenotype can be lost with the withdrawal of selective pressure [45]. Here, we have shown that the sensitivity of hFOB 1.19 to zinc is strongly affected by the presence of G418 both after short- and long-term incubation. We observed a higher sensitivity of hFOB1.19 to zinc in the absence of G418 (Figure 2). Some authors tend to use G418 not only during cultivation, but also during biomaterial tests [24,32,33] or the usage of G418 is not specified ([31,37]). In our opinion, in the case where the hFOB 1. 19 cell line is used as an appropriate cell model (mature osteoblastic phenotype is preferred, immortalization is not necessary), the G418 selection reagent does not need to be used during the experiment.

Furthermore, we studied the sensitivity hFOB 1.19 to zinc at different temperatures. We observed a higher sensitivity of hFOB 1.19 to Zn^{2+} at a restrictive temperature. Harris compared proliferation at 33.5 °C (as permissive), 38, and 39 °C (both considered restrictive). The doubling time

of hFOB 1.19 at 34 °C was ~36 h and at 38 °C it was > 96 h [20]. However, there is no clear consensus on whether the temperature of 37 °C should be considered permissive or restrictive. The higher metabolic activity and lower sensitivity to ZnCl₂ of hFOB 1.19 cells at permissive temperature (34 °C) in our case was probably due to their ongoing proliferation. The resulting cell density was higher and, therefore the concentration of Zn²⁺ per cell was lower. It is probably also due to the fact that at a temperature of 39.5 °C, the cells are stressed and thus more sensitive. This is supported by the fact that we observed an elevated level of heat shock proteins (HSP) in hFOB 1.19 at 39.5 °C (our unpublished results, [46]). In our opinion, the physiological temperature of 37 °C is ideal for the testing of biomaterials using the hFOB 1.19 cell line. HSP are probably not overexpressed and the temperature is sufficient for the development of the mature phenotype [20].

Comparison of the sensitivity of hFOB 1.19 to Zn²⁺ with the results obtained by other authors is difficult, since other studies using hFOB 1.19 to test degradable biomaterials with Zn (Table 1) do not specify the concentration of Zn²⁺ released to the medium in the contact with the cells.

We also compared the sensitivity of the hFOB 1.19 and L929 cell lines to Zn²⁺ (Figure 3). The higher sensitivity of L929 to Zn²⁺ compared to hFOB 1.19 is in agreement with our previous results showing that also another osteoblast-like cell line U-2 OS withstands a higher concentration of Zn²⁺ (200 μmol·l⁻¹, when tested in MEM medium) compared to the L929 fibroblast-derived cell line [47]. We did not compare hFOB 1.19 and U-2 OS directly, but from testing under the same conditions, we can presume that hFOB 1.19 are more sensitive than U-2 OS. Cell lines derived from bone cells (whether primary or cancerous) appear to be less sensitive to Zn²⁺ than the commonly used L929 line, and, therefore, their use in the testing of biomaterials intended for orthopedic implants may play a role in bringing the in vitro system closer to the real situation in the body.

We have also found that the type of media plays a prominent role. Our previous results showed that ZnCl₂ solutions were less toxic to L929 and U-2 OS in DMEM (Sigma, D0819) than in MEM (Sigma, M0446) [47]. This was confirmed for hFOB 1.19 (Figure 4), where the toxic effect of ZnCl₂ was lower in the case of rich DMEM/Ham's F-12 compared to minimal medium MEM. Surprisingly, ZnCl₂ was less toxic to L929 in MEM than in DMEM/Ham's F-12 (Figure 4). DMEM/Ham's F-12 is a mixture of component-rich Ham's F12 medium and the nutrient-rich DMEM medium. However, some of its components (e.g., ferrous sulphate, HEPES) may have negative effects on certain cell types [48]. It was also possible that L929 cells were unable to adapt to a new medium. Also, the availability of Zn in media can differ. For example, riboflavin (0.27 μmol·l⁻¹ in MEM vs. 1.0 μmol·l⁻¹ in DMEM/Ham's F-12) forms toxic complexes with certain metals [49].

We also prepared extracts of Zn-based biomaterials and tested the cytotoxicity of these extracts on the two cell types. The materials selected in the presented study are considered promising for future application in the development of medical devices. The chemical composition of these selected materials, especially its Mg content, is beneficial for improving mechanical strength and maintaining an adequate degradation rate of the materials [4,40,41,50]. The suggested processing by powder metallurgy (PM), including the preparation of alloy powder by mechanical alloying and its compaction by extrusion at 200 °C and an extrusion ratio equal to 25 enables the formation of extremely fine-grained homogeneous microstructures leading to superior mechanical properties and uniform degradation [42,43,51,52]. Silver is used particularly to improve materials' plasticity, but also the antibacterial and anti-inflammatory properties [53]. During the degradation process of alloy, silver is released into the surrounding tissue, where it fulfills the antibacterial effect and subsequently is gradually eliminated from the human body by the liver and kidney [54].

Extracts of the aforementioned materials were more toxic for L929 than for hFOB 1.19 (Figure 5). This is in agreement with the results with ZnCl₂ solutions (Figure 3). We prepared the extracts of the materials in both types of media. Generally, the extracts prepared in MEM were more toxic for the hFOB 1.19 cell line compared to the extract prepared in DMEM/Ham's F-12, even when they contained less Zn (Figure 5). Differences in media composition probably improved cell fitness and decreased the cytotoxic effect of extracts in DMEM/Ham's F-12 (rich medium) compared to MEM medium (minimal medium) similarly to our previous study with ZnCl₂ solutions in MEM and DMEM [47].

5. Conclusions

The human fetal osteoblast cell line hFOB 1.19 is a promising model for the in vitro testing of degradable zinc-based biomaterials intended for orthopedic applications due to its resemblance to primary osteoblasts and to its unlimited supply caused by conditional immortalization. The cultivation conditions during the testing can affect the results and should therefore be chosen with caution.

Author Contributions: Conceptualization: E.J., methodology: E.J. and J.L.; investigation: E.J. and L.M.; resources: J.K. and I.P.; writing—original draft preparation: E.J.; writing—review and editing: all authors; visualization: E.J.; supervision: J.L., T.R. and D.V.; project administration, J.K.; funding acquisition J.K. All authors have read and agreed to the published version of the manuscript.

Funding: This research was funded by The Czech Science Foundation (project no. 21-11439K).

Institutional Review Board Statement: Not applicable.

Informed Consent Statement: Not applicable.

Data Availability Statement: The datasets generated during and/or analyzed during the current study are available from the corresponding author on reasonable request.

Acknowledgments: We would like to thank Prof. Oto Mestek for ICP-MS analysis and to Dr. Markéta Častorálová for proof-reading and valuable comments.

Conflicts of Interest: The authors declare no conflict of interest.

References

1. Y.F. Zheng, X.N. Gu, F. Witte, Biodegradable metals, Materials Science and Engineering: R: Reports 77 (2014) 1-34.
2. D. Vojtěch, J. Kubásek, J. Šerák, P. Novák, Mechanical and corrosion properties of newly developed biodegradable Zn-based alloys for bone fixation, *Acta Biomater.* 7(9) (2011) 3515-3522.
3. I. Pospíšilová, D. Vojtěch, Zinc alloys for biodegradable medical implants, *Mater. Sci. Forum, Trans Tech Publ*, 2014, pp. 457-460.
4. J. Venezuela, M.S. Dargusch, The influence of alloying and fabrication techniques on the mechanical properties, biodegradability and biocompatibility of zinc: A comprehensive review, *Acta Biomaterialia* 87 (2019) 1-40.
5. H. Yang, B. Jia, Z. Zhang, X. Qu, G. Li, W. Lin, D. Zhu, K. Dai, Y. Zheng, Alloying design of biodegradable zinc as promising bone implants for load-bearing applications, *Nature Communications* 11(1) (2020) 401.
6. G. Katarivas Levy, J. Goldman, E. Aghion, The Prospects of Zinc as a Structural Material for Biodegradable Implants—A Review Paper, *Metals* 7(10) (2017).
7. I. Antoniac, R. Adam, A. Biță, M. Miculescu, O. Trante, I.M. Petrescu, M. Pogăreșteanu, Comparative Assessment of In Vitro and In Vivo Biodegradation of Mg-1Ca Magnesium Alloys for Orthopedic Applications, *Materials* (Basel) 14(1) (2020).
8. S. Janardhanan, M.O. Wang, J.P. Fisher, Coculture strategies in bone tissue engineering: The impact of culture conditions on pluripotent stem cell populations, *Tissue Engineering—Part B: Reviews* 18(4) (2012) 312-321.
9. G. Hulsart-Billström, J.I. Dawson, S. Hofmann, R. Müller, M.J. Stoddart, M. Alini, R. Redl, A. El Haj, R. Brown, V. Salih, J. Hilborn, S. Larsson, R.O.C. Oreffo, A surprisingly poor correlation between in vitro and in vivo testing of biomaterials for bone regeneration: results of a multicentre analysis, *European Cells and Materials* 31 (2016) 312-322.
10. G. Rijal, W. Li, Native-mimicking in vitro microenvironment: An elusive and seductive future for tumor modeling and tissue engineering, *J. Biol. Eng.* 12(1) (2018).
11. J.M. Anderson, Future challenges in the in vitro and in vivo evaluation of biomaterial biocompatibility, *Regenerative Biomaterials* 3(2) (2016) 73-77.
12. S. Ray, M.E. Anderson, G. Loeber, D. McVey, P. Tegtmeier, Functional characterization of temperature-sensitive mutants of simian virus 40 large T antigen, *J Virol* 66(11) (1992) 6509-6516.

13. I. Reynisdóttir, D. O'Reilly, L. Miller, C.J.J.o.v. Prives, Thermally inactivated simian virus 40 tsA58 mutant T antigen cannot initiate viral DNA replication in vitro, 64(12) (1990) 6234-6245.
14. ISO, Biological evaluation of medical devices, Part 5:Tests for in vitro cytotoxicity, 2009, p. 34.
15. C. Pautke, M. Schieker, T. Tischer, A. Kolk, P. Neth, W. Mutschler, S. Milz, Characterization of osteosarcoma cell lines MG-63, Saos-2 and U-2 OS in comparison to human osteoblasts, *Anticancer Res.* 24(6) (2004) 3743-8.
16. E.M. Czekanska, M.J. Stoddart, J.R. Ralphs, R.G. Richards, J.S. Hayes, A phenotypic comparison of osteoblast cell lines versus human primary osteoblasts for biomaterials testing, *J Biomed Mater Res A* (2013).
17. Y. Liu, T. Du, A. Qiao, Y. Mu, H. Yang, Zinc-Based Biodegradable Materials for Orthopaedic Internal Fixation, *Journal of functional biomaterials* 13(4) (2022).
18. W. Yuan, D. Xia, S. Wu, Y. Zheng, Z. Guan, J.V. Rau, A review on current research status of the surface modification of Zn-based biodegradable metals, *Bioactive Materials* 7 (2022) 192-216.
19. E. Jablonska, J. Kubasek, D. Vojtech, T. Rumí, J. Lipov, Test conditions can significantly affect the results of in vitro cytotoxicity testing of degradable metallic biomaterials, *Sci. Rep.* 11(1) (2021) 6628.
20. S.A. Harris, R.J. Enger, L.B. Riggs, T.C. Spelsberg, Development and characterization of a conditionally immortalized human fetal osteoblastic cell line, *Journal of Bone and Mineral Research* 10(2) (1995) 178-186.
21. M. Subramaniam, S.M. Jalal, D.J. Rickard, S.A. Harris, M.E. Bolander, T.C. Spelsberg, Further characterization of human fetal osteoblastic hFOB 1.19 and hFOB/ER alpha cells: bone formation in vivo and karyotype analysis using multicolor fluorescent in situ hybridization, *J. Cell. Biochem.* 87(1) (2002) 9-15.
22. M.-L. Yen, C.-C. Chien, I.-M. Chiu, H.-I. Huang, Y.-C. Chen, H.-I. Hu, B. Yen, Multilineage Differentiation and Characterization of the Human Fetal Osteoblastic 1.19 Cell Line: A Possible In Vitro Model of Human Mesenchymal Progenitors, *Stem cells* (Dayton, Ohio) 25 (2007) 125-31.
23. S. Marozin, B. Simon-Nobbe, S. Irausek, L.W.K. Chung, G. Lepperdinger, Kinship of conditionally immortalized cells derived from fetal bone to human bone-derived mesenchymal stroma cells, *Sci. Rep.* 11(1) (2021) 10933.
24. M. Cieslik, A. Mertas, A. Morawska-Chochól, D. Sabat, R. Orlicki, A. Owczarek, W. Król, T. Cieślik, The Evaluation of the Possibilities of Using PLGA Co-Polymer and Its Composites with Carbon Fibers or Hydroxyapatite in the Bone Tissue Regeneration Process—in Vitro and in Vivo Examinations, *Int. J. Mol. Sci.* 10 (2009) 3224-34.
25. K. Steckiewicz, E. Barcinska, A. Malankowska, A. Zauszkiewicz-Pawlak, G. Nowaczyk, A. Zaleska-Medynska, I. Inklelewicz-Stepniak, Impact of gold nanoparticles shape on their cytotoxicity against human osteoblast and osteosarcoma in in vitro model. Evaluation of the safety of use and anti-cancer potential, *J. Mater. Sci. Mater. Med.* 30 (2019).
26. M. Pallavi, J. Waterman, Y. Koo, J. Sankar, Y. Yun, In Vitro Cytotoxicity of Possible Corrosion Products from Mg-Based Biodegradable Metals: Magnesium Oxide and Magnesium Hydroxide Nanoparticles, *Applied Sciences* 9 (2019) 4304.
27. P.V. Gnaneshwar, S.V. Sudakaran, S. Abisegapriyan, J. Sherine, S. Ramakrishna, M.H.A. Rahim, M.M. Yusoff, R. Jose, J.R. Venugopal, Ramification of zinc oxide doped hydroxyapatite biocomposites for the mineralization of osteoblasts, *Materials Science and Engineering: C* 96 (2019) 337-346.
28. H.J. Donahue, Z. Li, Z. Zhou, C.E. Yellowley, Differentiation of human fetal osteoblastic cells and gap junctional intercellular communication, *Am J Physiol-Cell Ph* 278(2) (2000) C315-C322.
29. A. Oki, B. Parveen, S. Hossain, S. Adeniji, H. Donahue, Preparation and in vitro bioactivity of zinc containing sol-gel-derived bioglass materials, *Journal of Biomedical Materials Research Part A* 69A(2) (2004) 216-221.
30. L. Saidykhan, M.Z. Abu Bakar, Y. Rukayadi, A. Kura, S. Latifah, Development of nanoantibiotic delivery system using cockle shell-derived aragonite nanoparticles for treatment of osteomyelitis, *International journal of nanomedicine* 2016 (2016) 661-673.
31. V. Balla, A. Bhat, S. Bose, A. Bandyopadhyay, Laser Processed TiN Reinforced Ti6Al4V Composite Coatings, *J. Mech. Behav. Biomed. Mater.* 6 (2012) 9-20.
32. B. Setzer, M. Bächle, M.C. Metzger, R.J. Kohal, The gene-expression and phenotypic response of hFOB 1.19 osteoblasts to surface-modified titanium and zirconia, *Biomaterials* 30(6) (2009) 979-990.

33. G. Eugen, M. Claus, S. Anna-Maria, D. Niklas, S. Philipp, E. Andrea, M.-L. Andrea, V. Elke, Degradation of 3D-printed magnesium phosphate ceramics in vitro and a prognosis on their bone regeneration potential, *Bioactive Materials* 19 (2023) 376-391.
34. D. Predoi, S.L. Iconaru, M.V. Predoi, Fabrication of Silver- and Zinc-Doped Hydroxyapatite Coatings for Enhancing Antimicrobial Effect, *Coatings* 10(9) (2020) 905.
35. A. Donnadio, M. Bini, C. Centracchio, M. Mattarelli, S. Caponi, V. Ambrogi, D. Pietrella, A. Di Michele, R. Vivani, M. Nocchetti, Bioinspired Reactive Interfaces Based on Layered Double Hydroxides-Zn Rich Hydroxyapatite with Antibacterial Activity, *ACS Biomater. Sci. Eng.* 7(4) (2021) 1361-1373.
36. A. Laskus-Zakrzewska, P. Kazimierczak, J. Kolmas, Porous Composite Granules with Potential Function of Bone Substitute and Simvastatin Releasing System: A Preliminary Study, *Materials* 14(17) (2021) 5068.
37. I. Chirica, A.-M. Enciu, T. Teddy, M. Dudau, L. Albulescu, S.L. Iconaru, D. Predoi, I. Pasuk, M. Enculescu, C. Radu, C. Mihalcea, A.-C. Popa, N. Rusu, S. Niță, C. Tănase, G. Stan, The Physico-Chemical Properties and Exploratory Real-Time Cell Analysis of Hydroxyapatite Nanopowders Substituted with Ce, Mg, Sr, and Zn (0.5–5 at.%), *Materials* 14 (2021) 3808.
38. J. Higuchi, K. Klimek, J. Wojnarowicz, A. Opalińska, A. Chodara, U. Szałaj, S. Dąbrowska, D. Fudala, G. Ginalska, Electrospun Membrane Surface Modification by Sonocoating with HA and ZnO:Ag Nanoparticles—Characterization and Evaluation of Osteoblasts and Bacterial Cell Behavior In Vitro, *Cells* 11(9) (2022) 1582.
39. P. Kazimierczak, J. Golas, J. Kolmas, M. Wojcik, D. Kolodynska, A. Przekora, Noncytotoxic zinc-doped nanohydroxyapatite-based bone scaffolds with strong bactericidal, bacteriostatic, and antibiofilm activity, *Biomaterials Advances* 139 (2022) 213011.
40. J. Kubasek, D. Vojtech, E. Jablonska, I. Pospisilova, J. Lipov, T. Rumel, Structure, mechanical characteristics and in vitro degradation, cytotoxicity, genotoxicity and mutagenicity of novel biodegradable Zn-Mg alloys, *Mater Sci Eng C Mater Biol Appl* 58 (2016) 24-35.
41. J. Kubásek, J. Pinc, K. Hosová, M. Straková, O. Molnárová, J. Duchoň, D. Nečas, M. Čavojský, M. Knapek, M. Godec, I. Paulin, D. Vojtěch, J. Čapek, The evolution of microstructure and mechanical properties of Zn-0.8Mg-0.2Sr alloy prepared by casting and extrusion, *J. Alloy. Compd.* 906 (2022).
42. D. Nečas, J. Kubásek, J. Pinc, I. Marek, Č. Doník, I. Paulin, D. Vojtěch, Ultrafine-Grained Zn-Mg-Sr Alloy Synthesized by Mechanical Alloying and Spark Plasma Sintering, *Materials* 15(23) (2022) 8379.
43. D. Nečas, I. Marek, J. Pinc, D. Vojtěch, J. Kubásek, Advanced Zinc-Magnesium Alloys Prepared by Mechanical Alloying and Spark Plasma Sintering, *Materials* 15(15) (2022) 5272.
44. T.L. Riss, R.A. Moravec, A.L. Niles, S. Duellman, H.A. Benink, T.J. Worzella, L. Minor, Cell Viability Assays, in: G.S. Sittampalam, N.P. Coussens, B. K. (Eds.), *Assay Guidance Manual* 2016.
45. W. Liu, Y. Xiong, M. Gossen, Stability and homogeneity of transgene expression in isogenic cells, *J. Mol. Med.* 84(1) (2006) 57-64.
46. A. Ničová, Quantitative analysis of hFOB1.19 cell line proteome, The University of Chemistry and Technology, Prague, 2021.
47. E. Jablonská, J. Kubásek, D. Vojtěch, T. Rumel, J. Lipov, Test conditions can significantly affect the results of in vitro cytotoxicity testing of degradable metallic biomaterials, *Sci. Rep.* 11(1) (2021).
48. T. Yao, Y. Asayama, Animal-cell culture media: History, characteristics, and current issues, *Reprod. Med. Biol.* 16(2) (2017) 99-117.
49. Sigma-Aldrich, Riboflavin in Cell Culture. <https://www.sigmaaldrich.com/CZ/en/technical-documents/technical-article/cell-culture-and-cell-culture-analysis/mammalian-cell-culture/riboflavin>. (Accessed 21.3.2023 2023).
50. G. Chandra, A. Pandey, Biodegradable bone implants in orthopedic applications: a review, *Biocybernetics and Biomedical Engineering* 40(2) (2020) 596–610.
51. Z. Cui, M. Luo, Y. Zhang, D. Gong, W. Wang, J. Wang, Fabrication of high strength and plasticity of Zn-Mg composites with core-shell structure by spark plasma sintering, *Materials Letters* 279 (2020).
52. P. Sotoudeh Bagha, S. Khaleghpanah, S. Sheibani, M. Khakbiz, A. Zakeri, Characterization of nanostructured biodegradable Zn-Mn alloy synthesized by mechanical alloying, *J. Alloy. Compd.* 735 (2018) 1319-1327.

53. X. Xiao, E. Liu, J. Shao, S. Ge, Advances on biodegradable zinc-silver-based alloys for biomedical applications, *Journal of Applied Biomaterials & Functional Materials* 19 (2021) 22808000211062407.
54. A.B. Lansdown, Silver in health care: antimicrobial effects and safety in use, *Curr. Probl. Dermatol.* 33 (2006) 17-34.

Disclaimer/Publisher's Note: The statements, opinions and data contained in all publications are solely those of the individual author(s) and contributor(s) and not of MDPI and/or the editor(s). MDPI and/or the editor(s) disclaim responsibility for any injury to people or property resulting from any ideas, methods, instructions or products referred to in the content.