

Article

Use of Micropatterned Thin Film Nitinol in Carotid Stents to Augment Embolic Protection

Mahdis Shayan ¹, Brian T. Jankowitz ², Puneeth Shridhar ³ and Youngjae Chun ^{1,2,4,*}

¹ Department of Industrial Engineering, University of Pittsburgh, Pittsburgh, PA 15260, USA; mas461@pitt.edu

² Department of Neurological Surgery, University of Pittsburgh Medical Center, Pittsburgh, PA 15237, USA; btj1@pitt.edu

³ Department of Bioengineering, University of Pittsburgh, Pittsburgh, PA 15260, USA; pus8@pitt.edu

⁴ McGowan Institute for Regenerative Medicine, Pittsburgh, PA 15219, USA

* Correspondence: yjchun@pitt.edu; Tel.: +1-412-624-1193

Abstract: Stenting is an alternative to endarterectomy for the treatment of carotid artery stenosis. However, stenting is associated with a higher risk of procedural stroke secondary to distal thromboembolism. Hybrid stents with a micromesh layer have been proposed to address this complication. We developed a micropatterned thin film nitinol (M-TFN) covered stent designed to prevent thromboembolism during carotid intervention. This innovation may obviate the need or work synergistically with embolic protection devices. The proposed double layered stent is low-profile, thromboresistant, and covered with a M-TFN that can be fabricated with fenestrations of varying geometries and sizes. The M-TFN was created in multiple geometries, dimensions, and porosities by sputter deposition. The efficiency of various M-TFN to capture embolic particles was evaluated in different atherosclerotic carotid stenotic conditions through *in vitro* tests. The covered stent prevented emboli dislodgement in the range of 70-96% during 30min duration tests. *In vitro* vascular cell growth study results showed that endothelial cell elongation, alignment and growth behaviour silhouettes significantly enhance specifically on the diamond-shape M-TFN with the dimensions of 145µm×20µm and a porosity of 32%. Future studies will require *in-vivo* testing. Our results demonstrate that M-TFN has a promising potential for carotid artery stenting.

Keywords: thin film nitinol; carotid artery; micro mesh stent; micropatterning

1. Introduction

Approximately 795,000 people suffer from a stroke annually in the U.S. and 15-20% of these strokes are associated with carotid artery disease [1, 2]. These strokes are likely due to a combination of hypoperfusion from stenosis and distal thromboembolism. Carotid endarterectomy (CEA) is the gold standard treatment option for carotid artery stenosis [2]. However, carotid artery stenting (CAS) has become an increasingly popular alternative with recent evidence supporting its equivalence to CEA [3].

CAS consistently shows a higher risk of procedural stroke which is likely due to an increased risk of distal thromboembolism, particularly during angioplasty. Various types of embolic protection devices (EPDs) have been designed to reduce this risk [4]. While the use remains logical and compelling, no randomized studies have been able to prove the efficacy of EPDs [5].

All currently Food and Drug Administration (FDA) approved carotid stents are bare metal, single layer, and have a large pore size. Due to the procedural risk of distal thromboembolism, from atherosclerotic debris extruding through the stent pores, there is currently significant interest in creating a covered stent to trap debris against the blood vessel wall. The cover would optimally

need to be porous so it does not occlude side branches such as the external carotid artery. Recently, a CE-marked covered stent, CGuard™ system, consisting of metallic stent covered with an ultra-thin polyethylene terephthalate (PET) mesh has been studied. A 30-day clinical trial in patients undergoing carotid artery stenting with CGuard™ system demonstrated the safety and efficacy of this device [6]. Another promising stent called Roadsaver™ made up of an ultra-thin nitinol wire micromesh woven onto an external closed-cell stent to achieve a cell size of 375 to 500 μm has been recently gaining traction [7]. In both stent frames, the micromesh or double layer technology aims at preventing plaque protrusion [8]. New stent designs incorporating an inner mesh with pore sizes down to below 200 μm may allow additional reduction of lesion-derived microemboli [9]. The current generation carotid stents typically incorporate an open or closed-cell design. Open-cell stents have better conformability and wall apposition but their larger pore size reduces plaque coverage and allows a higher risk of debris extrusion [10]. Recent imaging capabilities like Optical Coherence Tomography (OCT) have played an important role in identifying the plaque prolapse [11]. The closed-cell stents have superior scaffolding and plaque coverage due to their smaller pore size however this increases the probability of mal-apposition, especially within tortuous arteries [12]. A hybrid configuration with an open-cell design at the proximal and distal ends combined with a closed-cell design of the central segments has been recently developed. It not only allows greater apposition to the vessel wall but also offers improved plaque coverage.

In this study, we employ micropatterned thin film nitinol as the covering membrane for a double layer carotid stent. Thin film nitinol (TFN) is a novel material worth considering for developing a low-profile endovascular device [13]. Vacuum sputter deposition process for thin film nitinol is the preferred fabrication method because of the precise controllability of the deposition process and the consistency of the quality of the films [14]. Furthermore, thin film nitinol can be used in small calibre vascular systems as it exhibits superelastic property at body temperature, which improves the device apposition to the vascular wall compared to any synthetic fabric (like polyethylene terephthalate micronet) that typically has wrinkles or permanent deformation.

In vitro studies were performed to evaluate the feasibility of micropatterned thin film nitinol as a carotid stent cover. We specifically looked at this new stent's ability to capture embolic particles and inhibit distal embolization of artificial plaque debris. We also studied its interaction with endothelial cells.

2. Materials and Methods

2.1. Preparation and Characterization of micropatterned thin film nitinol (M-TFN)

The sputter deposition technique along with a lift-off process previously described by Chun *et al* was used to create M-TFN [15]. First, five different micro patterns were defined via a conventional photolithography process. Then, 50 μm deep trenches were created by Deep Reactive Ion Etching (DRIE) technique. Once trenches were formed, both copper sacrificial layer and silicon dioxide material inhibition layer were deposited for thin film nitinol sputter deposition process. The deposited thin film nitinol was crystallized at 500°C for 20min in a vacuum of less than 1×10^{-7} Torr [16]. Finally, the M-TFN was obtained by etching sacrificial and inhibition layers consecutively. Scanning electron microscopy (SEM) (Jeol-JSM 6610 LV, Japan) was used to characterize the geometry and size of the M-TFN. The obtained SEM images were used to calculate the porosity of

the fenestrations in M-TFN with the custom-built MATLAB R2015a (MathWorks, MA) image analysis code.

2.2. *In Vitro* Testing for Assessing the Efficiency of Embolic Protection Capability

Figure 1A shows a bench-top flow loop equipped with a pulsatile pump used for the *in vitro* testing for assessing the efficiency of embolic protection capability of the five different M-TFN covering membranes. This test apparatus consists of platinum cured silicone tubing (Cole-Parmer, IL) with inner diameter of 6.5mm, which is close to the average human carotid artery dimensions [17]. In order to mimic the carotid artery stenosis we used fluorescent microspheres (Cospheric, CA) with different dimensions (e.g., diameter in the range of 53–63µm) along with the water-soluble polyvinyl alcohol (PVA) glue (Lineco Inc., MA). Microspheres in two different weight loads (*i.e.*, 10mg and 30mg) were homogenously dispersed in 500mg PVA fluid. The PVA fluid that contains microspheres was uniformly deposited on the luminal side of the silicone tubing. The total length of the deposition was determined to be 14mm based on the longitudinal length of the M-TFN covering membrane used for the experiment. Then, M-TFN covering membrane was rolled and collapsed into a 6Fr delivery catheter with the commercially available bare metal stent (PFM Medical, Germany). The PFM medical stent was used only for exerting the radial force to the M-TFN under *in vitro* testing. Other commercially available stents, such as Acculink (Abbott Laboratories, IL), Precise (Cordis Corporation, FL), or Xact (Abbott Laboratories, IL) stents should be used for future *in vivo* animal testing (not in this study). The stent was deployed on the microsphere mixed PVA fluid covering the strut with the M-TFN membrane, which mimics the embolic protection device of the covered stent. Once the artery models were prepared, these were submerged in the 37°C water bath, then, connected to the pulsatile flow pump (Harvard apparatus, MA). The blood mimicking solution (viscosity of 3.4cP by mixing DI water and Glycerol) [18] was applied to achieve realistic circulation of the flow, which circulated at 402 and 510mL/min and 65 and 85 beats per minute (bpm) in the tube for 30min [19]. Both flowmeter (FLR1000, Omega, CT) and pressure sensor (PressureMAT, PendoTECH, NJ) were integrated adjacent to the carotid artery model to monitor the flow and pressure conditions in a real time. At the end of the flow loop, a micromesh filter (Component Supply Co Inc., FL) with 105µm pore dimension (32% opening area) was placed to collect the dislodged microspheres from the wall of the artery model. The microspheres collected by the filter were characterized using a fluorescent microscopy system (Olympus BX43, Olympus Co, Tokyo, Japan) to mimic and quantify the amount of the dislodged emboli under the typical carotid artery ischemic disease conditions.

2.3. *In Vitro* Cell Culture Experiment

Both non-patterned thin film nitinol (*i.e.*, control sample) and M-TFN were prepared with the dimension of 1cm×1cm. All samples were sterilized by immersion in 70% ethanol for 30min, then, transferred to a 12-well tissue culture plate (Becton Dickinson and company, NJ). After transferring the samples to a culture plate, all samples were washed with sterile PBS (Gibco, NY). BAEC (Bovine Aortic Endothelial Cells; Lonza, NJ) at passage number 5 were seeded at a density of 2×10^5 cells/cm² on the samples. Cells were grown in the cell culture medium consisting of Endothelial Cell Basal Medium (EBM)-2 (Lonza, NJ) and EGM-2 SingleQuot Kit Suppl. & Growth Factors (Hydrocortisone

0.02%, FBS2%, VEGF0.05%, hFGF-B2%, IGF-1 0.05% and HEGF 0.05%, GA-1000 0.05%) (Lonza, NJ). A 2 ml cell culture medium was added in each well of the tissue culture plate and the plates were kept in a humidified incubator under 5% CO₂ at 37°C.

In order to visualize the cell morphology, Alexa Fluor® 488 Phalloidin (Thermo Fisher scientific, PA) was used for the staining of F-actin. After 48hrs of cell culture, the samples were washed with PBS, fixed in 3.7% formaldehyde solution in PBS for 10 min at room temperature and then each sample was extracted using acetone at -20°C for 3-5min. Subsequently, the samples were loaded with the fluorescent Phalloidin and washed with PBS, and then, images were taken using fluorescent microscopy.

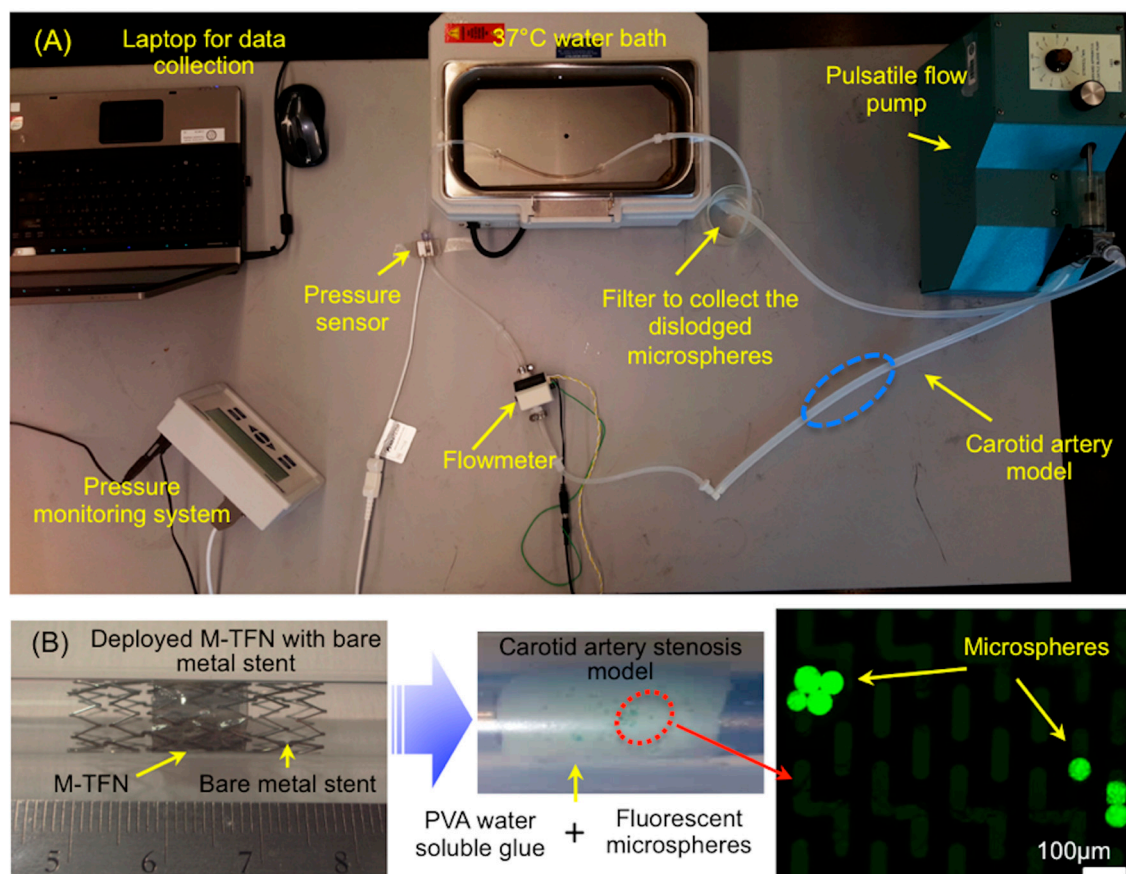


Figure 1. A) In vitro flow loop for assessing the M-TFN covered stent's performance and B) Deployed M-TFN with a commercially available bare metal stent (left), PVA based water-soluble glue layer with fluorescent microspheres (middle), and microspheres characterized by microscopy (right).

2.4. Endothelial Cell Growth Behavior Study

2.4.1. Quantification of Endothelial Cell Elongation and Alignment

To quantitatively evaluate the cell elongation and orientation, each Phalloidin stained cell was visualized as an elliptical shape. The ratio of the major elliptic axis of the individual stained cells with respect to the horizontal axis was measured using MATLAB R2015a (MathWorks, MA) image analysis. In addition, the angle between the major axis of each individual cell with respect to the long axis of the micropatterns was measured as the alignment angle using MATLAB image analysis. Four random locations were characterized for both five M-TFN samples and control (i.e., nonpatterned film) samples for the analysis (i.e., total 24 images).

2.4.2. MTT Endothelial Cell Viability and Proliferation Assay

Cell proliferation was assessed by a colorimetric assay using 3-(4, 5-dimethylthiazol-2-yl)-2, 5-diphenyl tetrazolium bromide (CT02 MTT Cell Growth Assay Kit: EMD Millipore, Darmstadt, Germany). Cells were cultured for 1hr, 4hrs, 24hrs and 5 days at an initial seeding density of 2×10^5 cells/ml on both M-TFN and control samples with three replicates of each sample. After determining the incubation time, 0.01ml pre-warmed MTT solution containing 0.1ml fresh cell medium was added to each culture well, then, continuously incubated for 4hrs under the same conditions. After 4hr incubation of cells with MTT, 0.1ml isopropanol with 0.04 N hydrochloric acid (HCl) was added to each well. The HCl converts the phenol red in tissue culture medium to a yellow colour that does not interfere with MTT formazan measurement. The isopropanol dissolves the formazan to give a homogeneous blue solution. The absorbance was measured at a wavelength of 570nm using microplate reader (BioTek Synergy 2, VT).

2.4.3. Morphology and Coverage Percentage of Endothelial Cells

The morphology of the endothelial cells adhered on each sample was characterized by SEM after a thin layer of palladium deposition by sputtering. For the SEM, cells were fixed with 2.5% glutaraldehyde (Sigma-Aldrich, MO), dehydrated in a series of ethanol/DI water mixtures including 30%, 50%, 75%, 90% and 100% ratios, then, subjected to drying with hexamethyldisilazane (HMDS) (Alfa Aesar, MA, USA)/ethanol in 3:1, 1:1 and 1:3 volume ratios. The samples were then dried in the hood overnight at room temperature. Coverage percentage of endothelial cells on the M-TFN and the control samples were analysed using MATLAB image analysis based on the SEM images.

2.5. Statistical Analysis

The values related to the embolic protection efficiency of the M-TFN, optical density with respect to MTT assay, aspect ratio of attached endothelial cells and endothelial cell coverage percentage were expressed as the mean value \pm standard deviation (SD). Statistical analysis was performed for the experiment using one-way analysis of variance (ANOVA) test and Tukey's HSD test by Minitab® 16.1.0 statistical software (Minitab Inc. PA) and a P-value < 0.01 was considered to be statistically significant.

3. Results and Discussion

3.1. Efficiency of the Embolic Protection Capability (EEPC) of the M-TFN Covered Stents

Table 1 shows the parameters selected for *in vitro* embolic protection capability study of the M-TFN stents based on the carotid artery stenosis environment described in Section 2.2.

Table 1. Parameters used for assessing the efficiency of embolic protection capability (EEPC).

Number	Flow rate (ml/min)	Pulsatile rate (beats per min)	Weight of microspheres (mg)	PVA Solution (mg)	Particle Size (µm)
1	510	85	30	500	53-63
2	402	65	30	500	53-63
3	510	85	10	500	53-63
4	402	65	10	500	53-63

Figure 2A and 2C show the scanning electron microscopy (SEM) images of two different fenestrations with elliptical geometry. The first micropattern (Figure 2A) had a lateral length of 118µm and vertical length of 38µm. The porosity of first M-TFN sample was 44%. The second ellipse (E) micropattern had a lateral length of 98µm and vertical length of 23µm, showing 39% of porosity. While both E-patterns have different pore size and porosity, the embolic protection efficiencies were found to be very similar.

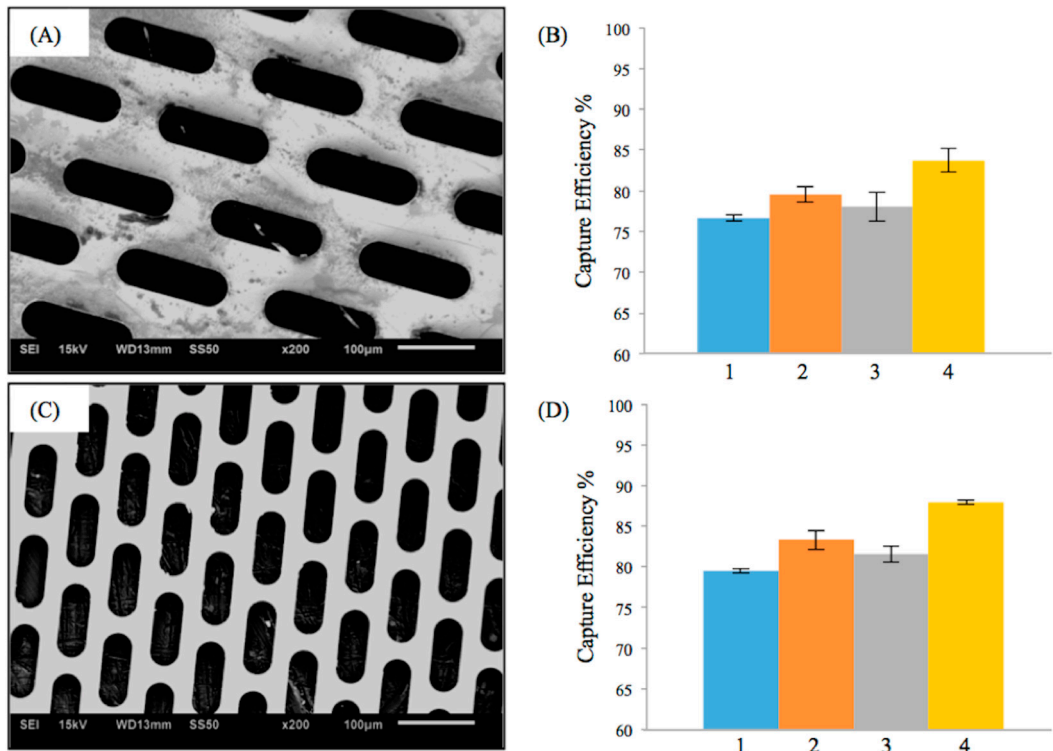


Figure 2. Results on the efficiency of embolic protection with two different size of ellipse patterns in thin film nitinol; (A) and (B) show the fenestration size of 118 x 38 µm, (C) and (D) show the fenestration size of 98 x 23 µm

Figure 2B and 2D represent the efficiency of the embolic protection capability, i.e., the percentage of the number of particles isolated by M-TFN covering membrane compared with the

total number of particles. The particles left on the wall of carotid artery model by the first pattern of M-TFN were seen to decrease with the higher flow rates (i.e., conditions 1 and 3 in Figure 2B). The higher flow rates in the same diameter artery model resulted in an increase in the flow velocity as well as shear rate on the wall of the model. Therefore, condition 1 had less number of particles left on the wall showing almost similar EEPC of 76.65% and 79.48%, respectively. Condition 3 also showed EEPC of 78.02% and 81.52% in each sample, respectively. The highest EEPC among both E-patterned samples were found in condition 4 showing 83.74% and 87.94%, respectively.

Similar trends as in M-TFN with E-patterns were found in M-TFN with diamond shaped (D) micro patterns. Figure 3A and 3C show two different types of D-patterns created in TFN. The first pattern (Figure 3A) has 32% porosity with a lateral length of 145 μ m and vertical length of 20 μ m. The second pattern (Figure 3B) has 17% porosity with a lateral length of 55 μ m and vertical length of 30 μ m. Similar to EEPC seen in E-patterns, higher flow rates resulted in the decrease in EEPC for the first D-pattern (Figure 3B). However, the EEPCs were very similar for the D-patterned TFN with 17% of porosity. Compared with the E-patterns, D-patterns showed better EEPC with slightly decreased porosity. For example, while the second E-pattern (Figure 2C) with 39% porosity showed EEPC of 79.49, 83.30, 81.52, and 87.94% for the conditions from 1 to 4, respectively, the first D-pattern (Figure 3A) with 32% porosity showed EEPCs of 85.01, 89.02, 85.48, and 89.77%. Also, it was noted that M-TFN with much less porosity showed higher EEPCs indicating 92.67, 94.59, 93.25, and 94.95% for the conditions from 1 to 4, respectively.

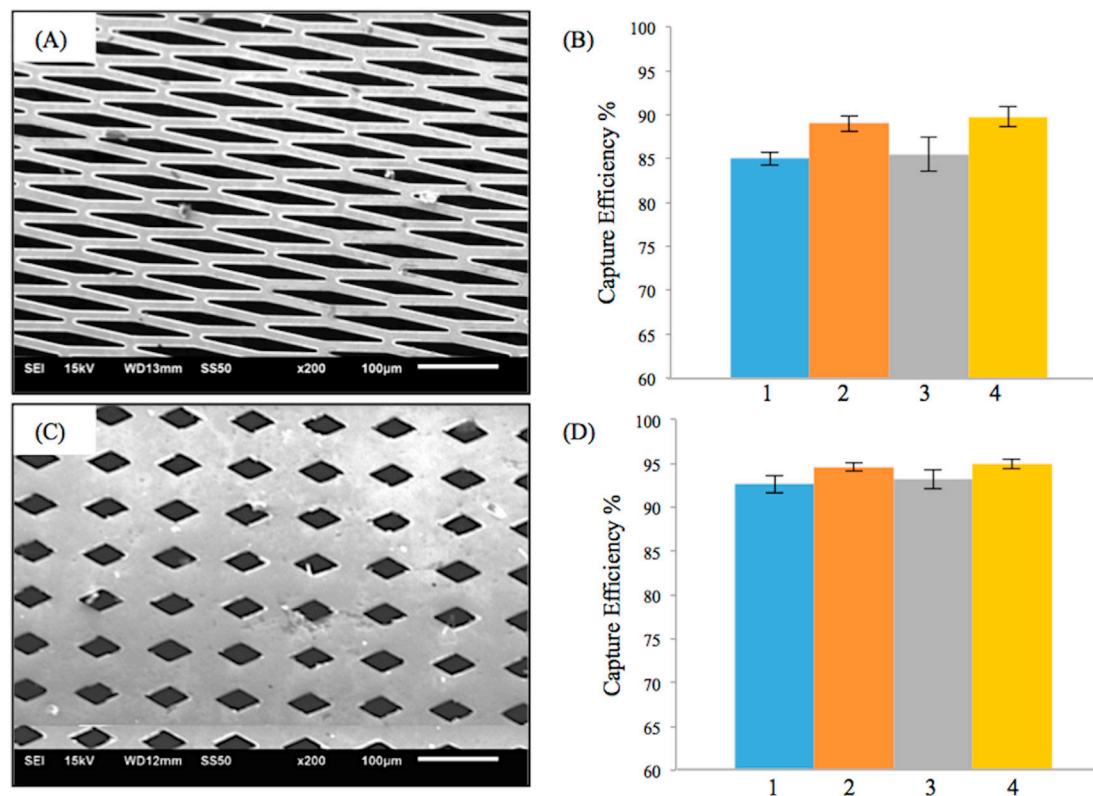


Figure 3. Results on the efficiency of embolic protection with two different size of diamond patterns in thin film nitinol; (A) and (B) show the fenestration size of 145 x 20 μ m, (C) and (D) show the fenestration size of 55 x 30 μ m

Figure 4A shows the SEM image of the M-TFN with circular (C) patterns with the diameter of 5 μ m. The porosity of C-pattern was 15%, which was slightly less than the porosity found in the low

porosity D-patterns (Figure 3C). The EEPs showed very similar trend as observed in D-patterns (Figure 3D). The C-pattern showed EEPs 94.36, 95.61, 93.15, and 96.18% for the conditions from 1 to 4, respectively. There was no significant difference between the two samples, i.e., Figure 3D and 4B, representing the low porosity below ~17% which does not actually represent an increase in the EEP. In addition, we may note that the M-TFNs with lower porosity (Figure 3C and 4A) exhibit longitudinal stiffness, as well as such patterns are virtually impossible to be collapsed into a small delivery catheter. Therefore, the optimal micro pattern will be the D-pattern with flexible TFN, which is represented as in Figure 3A.

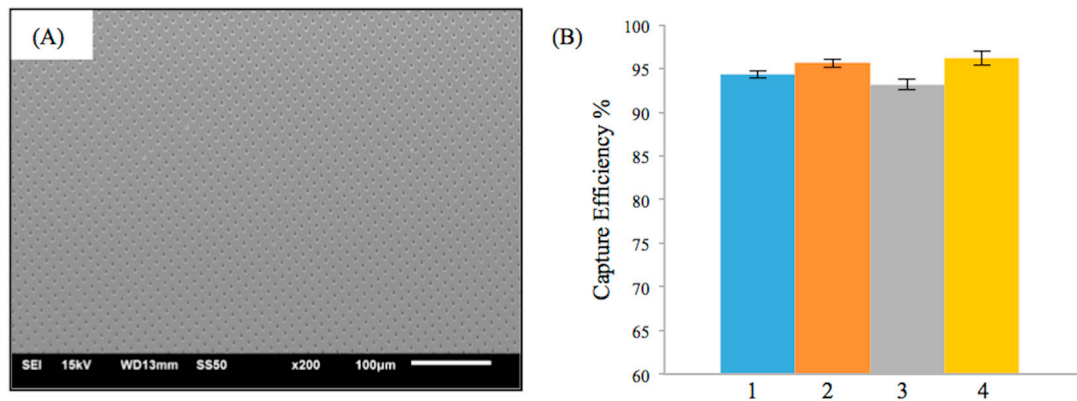


Figure 4. Results on the efficiency of embolic protection with circular pattern in thin film nitinol; (A) and (B) show the fenestration size of 5 µm in diameter.

3.2. Biocompatibility Assessment via In Vitro Endothelial Cell Growth Behavior

Biocompatibility of M-TFN as a covering membrane for carotid stent should be evaluated to demonstrate efficacy of the material in use. In this study, endothelial cell growth behaviour studies were conducted to assess (1) cell viability and proliferation with TFN using MTT assay, (2) the shape of the grown cells on TFN using both fluorescent microscope and scanning electron microscope image analyses, (3) the orientation of cells grown on TFN, and (4) the morphologies of the grown cells on TFN. The D-pattern in Figure 3A was chosen for endothelial cell growth behaviour studies because this pattern showed appropriate EEP as well as flexible device design capabilities.

Figure 5 represents the mean value of endothelial cell's viability on TFN and M-TFN samples that were evaluated using the MTT assay over five different time periods (1hr, 2hrs, 4hrs, 1day and 5 days). After 1hr, 2hrs, 4hrs and 1 day, no significant difference in optical density was observed between the TFN and M-TFN samples. After 5 days, however, the optical density was seen to be on the rise on M-TFN sample (value = 0.2273). It was 18.38% higher compared with the density found in nonpatterned TFN (value = 0.192). Overall, our short term in vitro tests showed better endothelial cell proliferation performance in M-TFN rather than non-patterned TFN (p-value<0.01).

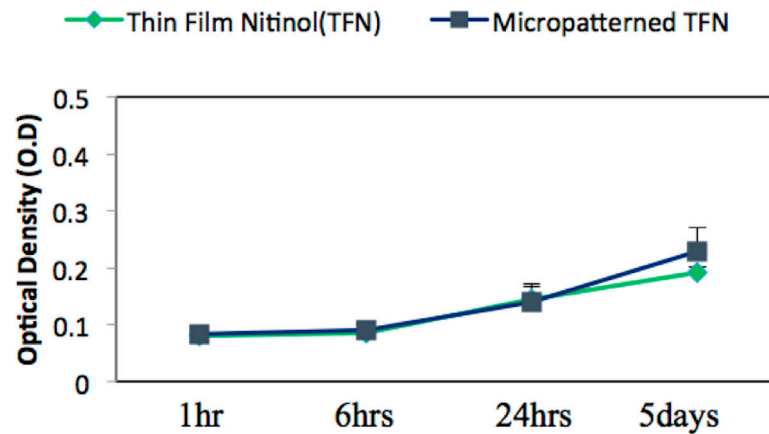


Figure 5. MTT assay for endothelial cell viability cultured on the TFN and micropatterned TFN substrates after 1 hr, 2 hrs, 4 hrs, 24 hrs and 5 days.

3.3. Quantification of the Endothelial Cell's Growth Pattern and Orientation

Figure 6 shows the representative fluorescent images of stained endothelial cells cultured on (A) TFN and (B) M-TFN after 48 hrs. As illustrated in Figure 5, MTT assay showed more endothelial cells adhered on the M-TFN along the line of the micro patterns in TFN. The scale bars are depicted in 50 μ m. Figure 6C shows the aspect ratio (i.e., ratio of the minor axis to the major axis) of the cells found on the films. The aspect ratio of 1 would mean a symmetric geometry in x- and y- axis. Therefore, as illustrated in Figure 6C, M-TFN showed longer shape of cells with 0.232 aspect ratio compared with non patterned TFN (0.479), indicating endothelial cells have a tendency to grow along the line of TFN.

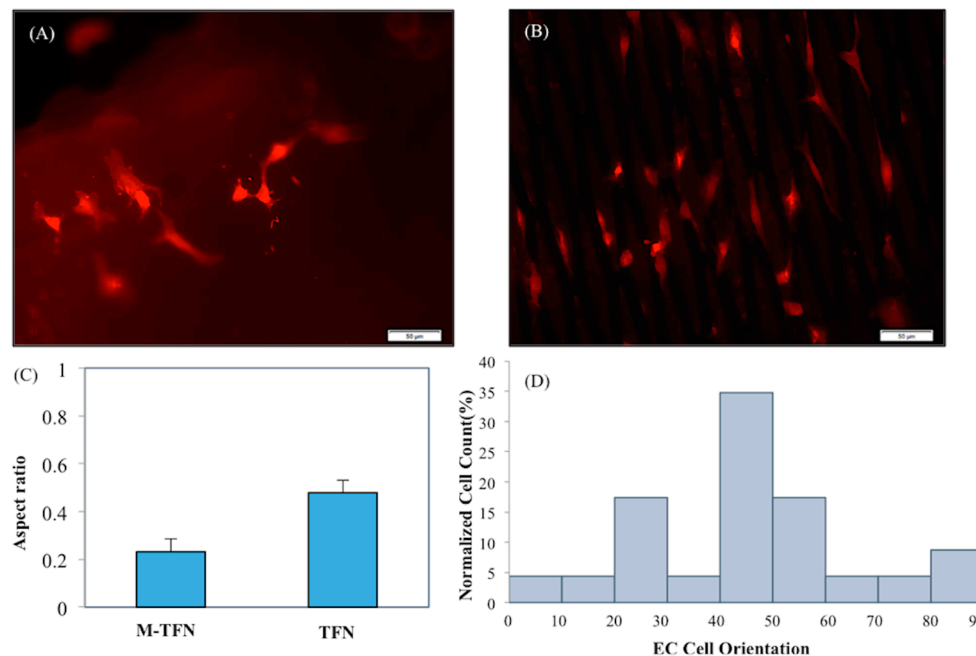


Figure 6. Representative Fluorescent images of F-actin stained endothelial cell cultured on (A) TFN, (B) M-TFN after 48 hrs, (C) aspect ratio of the grown endothelial cells on TFN and M-TFN, and (D) orientation angles of the endothelial cells grown on TFN and M-TFN after 48 hrs.

Figure 6D shows the distribution of alignment angles of endothelial cells along the major axis of

M-TFN. Quantitative analysis of actin alignment of endothelial cells on the M-TFN showed that approximately 35% of cells were oriented along the major axis of the micro patterns with the angle of 40-50°. Almost 17% of cells were grown with 20-30° and 17% with 50-60° orientations. This finding shows the endothelial cells on M-TFN were grown along the line of TFN area supporting the observations derived from Figure 6C.

3.4. Morphology and Coverage Percentage of Endothelial Cells

Figure 7 shows the representative SEM images of endothelial cells cultured on both TFN and M-TFN. Endothelial cells are seen spread out on the TFN substrate and major podia have emerged on the surface of cells (Figure 7A). For M-TFN samples, as in Figure 7B, a few cells were observed on TFN area and more aggregated endothelial cells were found in the middle demonstrating that porous regions are also covered with cells over time. The number of grown cells were counted with the SEM images. Figure 7D shows higher number (120%) of grown endothelial cells in M-TFN compared with TFN. In general, the M-TFN exhibits higher surface-to-volume ratio, therefore, there are increased tendency for cells to adhere on this sample. In addition, micro patterns actually enhance the cell growth behaviour by providing complex structure where cells are more easily attached.

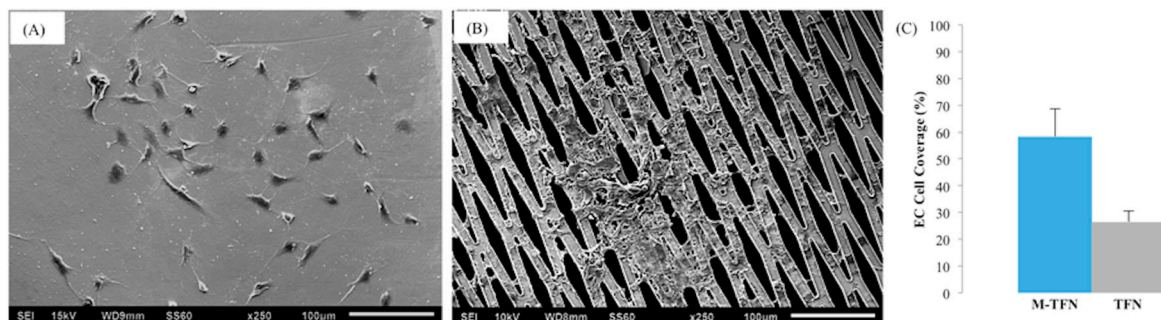


Figure 7. Representative SEM images of endothelial cells cultures on (A) TFN and (B) M-TFN, and (C) percentage of endothelial cells covered on M-TFN and TFN samples..

Covered stents are an attractive way to treat carotid artery stenosis. Following promising results from small case series, a prospective multicentre European trial (Clear Road Trial) showed that the multi-layered Roadsaver™ stent is safe and effective in high risk subjects for carotid endarterectomy [21]. Another multi-centre CAS study with 150 patients showed a lower rate of plaque prolapse and favourable short term outcome [22]. The increased pore density of “mesh stents” promise even higher plaque containment by either avoiding, or at least limiting, plaque prolapse through the cell struts [23].

Thin film nitinol is a promising candidate for use in endovascular devices [24]. It's super low profile minimizes interruption of the vascular lumen and would not disturb the blood flow. It maintains superior versatility compared to micromesh technology. Kedev *et al.* suggested that it is possible that the unique double-layer micromesh design of these stents may obviate the need for systematic embolic protection [25]. However, recent clinical studies like Confidence Trial have been designed to include both dual layer stents and embolic protection devices (e.g. Nanoparasol).

Covered stent for preventing embolization in carotid artery stenosis would be ideal because the stent can physically isolate the embolic particles without any additional filter devices or complex

steps of procedures. However, a covered stent is not flexible enough to be delivered in some tortuous locations, as well as they add bulkiness, which may possibly complicate its delivery in an endovascular procedure. In addition, fenestrations should be present in the overlying covering membrane to allow nutrition and oxygen transport from the blood stream to the cells on the wall of the vascular system.

In this study, we introduced a novel covering membrane material, i.e., thin film nitinol. The thin film nitinol has 6 μ m thickness, and thus could be an ideal candidate for use in low-profile devices for carotid artery stenosis. In addition, various shapes and sizes of pores can be created in the thin metallic film using a lift-off process. As a carotid embolic protection stent, we have showed the relationship among the efficiency of embolic protection, the geometry, and size of micro-sized patterns created in thin film nitinol. We have demonstrated that thin film nitinol covering membrane patterned in various morphologies (i.e., ellipse, diamond and circle) with different porosities (i.e., 44, 39, 32, 17, and 15%) can isolate embolic particles efficiently (\sim 75%) during a 30min *in vitro* flow test. In our tests, lower flow rates resulted in the increase in capture efficiency or efficiency of embolic protection capability. Furthermore, lower porosity was conducive to improve the efficiency of embolic protection capability. We believe there is a lower limit for porosity below which no improvement in EEPC may be seen. Among circular (C), diamond (D), elliptical (E) shaped micro-patterns, the diamond shape with a lateral length of 145 μ m and vertical length of 20 μ m (D-pattern in Fig. 3A) is the most favourable in terms of embolic protection efficiency. Also, smaller micro patterns increase the stiffness of the collapsed stent, or even to the extent of not being collapsible into a small delivery catheter.

One other important design criteria for the success of the carotid artery stent is the reduction of the risk of thrombosis and restenosis occurrence which are two major complications leading to the failure of the endovascular devices [26-30]. During a restenosis event, arterial lumen is narrowed again due to the migration of smooth muscle cells and thickening of the scar tissue. Growing a layer of healthy endothelial cells on the thin film nitinol cover and stent struts not only develops a normal lining allowing the normal blood flow, but it also reduces the probability of thrombosis or neointimal hyperplasia. This is achieved by formation of a native vascular endothelium that protects the vessel wall from smooth muscle cell migration and proliferation as well as inflammatory cell infiltration [31].

A number of studies have shown that endothelial cellular response (e.g., adhesion, proliferation) favourably changes on the micro-patterned substrate [32, 33]. It is now well-known that micropatterned substrates can significantly modulate cellular responses [34-36]. In the case of the smooth surface of a biomaterial substrate (e.g., TFN), cells encounter a homogenous substrate which does not have many important features of the native tissue microenvironment. In the native tissues, each cell is normally surrounded by neighbouring cells within an extracellular matrix (ECM) that constitutes the 3D microenvironment imposing both geometrical and topographical constraints. The ECM ligands binding with the cell surface receptors not only affect the intracellular signalling pathways, they can also impact the cytoskeleton architecture e.g., actin network, cell polarity, migration, differentiation and growth.

In our study, *in vitro* results demonstrated that more than twice the endothelial cell coverage can be seen on micropatterned thin film nitinol compared to the nonpatterned thin film nitinol surface. Also, our short term endothelial cell proliferation test results point in the direction of

M-TFN when compared to non patterned TFN. The alignment and orientation is related to cytoskeleton organization *e.g.*, actin aligning and it plays a very important role in the cellular function like cell proliferation [37, 38]. The majority of the endothelial cells are aligned at an angle of 40-50° along the axis of the micropatterns. In theory, M-TFNs have higher surface-to-volume-ratios compared to nonpatterned TFNs. We have demonstrated this holds true in our case. This property is particularly useful and ideal to enhance cell growth behaviour in micromesh carotid stents. However, more studies are needed to find out the longer term relationship between the endothelial cell shape and its functional behaviour, as well as *in vivo* tests.

4. Conclusions

We have shown that micropatterned thin film nitinol based covered stents are promising biomaterials for the fabrication of dimensionally and geometrically well-defined, carotid artery stents. The effective geometric properties (especially diamond shaped patterns) and the porosities of the micropatterned thin film substrate can be extremely important to improve the efficiency of the embolic prevention. This capability, in turn, improves the stroke prevention profile of the carotid stent and obviates the requirement of embolic protection devices. The micropatterned TFNs are highly biocompatible. The elongation, alignment, viability, and proliferation of the endothelial cells, along with the morphology and coverage, are controlled by the presence of micropatterns in the TFN substrate. All these properties together highlight the suitability of the micropatterned thin film nitinol for hybrid carotid stents for endovascular applications, where the material must be able to prevent both early and late embolization without blocking side arteries and exhibit high flexibility to ensure easy deployment for the utility during an intervention. *In vivo* studies must be carried on to demonstrate whether these preliminary results might translate into relevant clinical benefits as compared to the current available technologies.

Acknowledgments: The authors most gratefully appreciate funding provided for this work by the National Institute of Neurological Disorders and Stroke (NINDS) of the National Institutes of Health under Grant 5R03NS083956-02.

Author Contributions: Mahdis Shayan and Youngjae Chun have jointly written the paper.

Conflicts of Interest: The authors declare no conflict of interest.

References

1. Foulkes MA, Wolf PA, Price TR, Mohr JP, Hier DB. The Stroke Data Bank: design, methods, and baseline characteristics. *Stroke*. 1988;19(5):547-54. [[CrossRef](#)] [[PubMed](#)]
2. Thom T, Haase N, Rosamond W, Howard VJ, Rumsfeld J, Manolio T, et al. Heart disease and stroke statistics--2006 update: a report from the American Heart Association Statistics Committee and Stroke Statistics Subcommittee. *Circulation*. 2006;113(6):e85. [[CrossRef](#)] [[PubMed](#)]
3. Mantese VA, Timaran CH, Chiu D, Begg RJ, Brott TG, Investigators C. The carotid revascularization endarterectomy versus stenting trial (CREST) stenting versus carotid endarterectomy for carotid disease. *Stroke*. 2010;41(10 suppl 1):S31-S4. [[CrossRef](#)] [[PubMed](#)]
4. Kastrup A, Gröschel K, Krapf H, Brehm BR, Dichgans J, Schulz JB. Early outcome of carotid angioplasty and stenting with and without cerebral protection devices a systematic review of the literature. *Stroke*. 2003;34(3):813-9. [[CrossRef](#)] [[PubMed](#)]

5. Stone GW, Webb J, Cox DA, Brodie BR, Qureshi M, Kalynych A, et al. Distal microcirculatory protection during percutaneous coronary intervention in acute ST-segment elevation myocardial infarction: a randomized controlled trial. *Jama*. 2005;293(9):1063-72. [[CrossRef](#)] [[PubMed](#)]
6. Rosamond W, Flegal K, Furie K, Go A, Greenlund K, Haase N, et al. American heart association statistics committee and stroke statistics subcommittee. Heart disease and stroke statistics—2008 update: a report from the American Heart Association Statistics Committee and Stroke Statistics Subcommittee. *Circulation*. 2008;117(4):25-146.
7. Castagno C, Varetto G, Sperti F, Rossato D, Faletti R, Rispoli P. Preoperative and Postoperative Evaluation of New Double Mesh Carotid Stents with Contrast-Enhanced Ultrasound and Diffusion-Weighted Imaging. *Annals of vascular surgery*. 2016;33:228-9. [[CrossRef](#)] [[PubMed](#)]
8. Ruffino MA, Faletti R, Bergamasco L, Fonio P, Righi D. Incidence of New Ischaemic Brain Lesions After Carotid Artery Stenting with the Micromesh Roadsaver Carotid Artery Stent: A Prospective Single-Centre Study. *CardioVascular and Interventional Radiology*. 2016:1-9. [[CrossRef](#)]
9. Mudra H, Staubach S, Hein-Rothweiler R, Segerer M, Strohm H, Weber H, et al. Long-Term Outcomes of Carotid Artery Stenting in Clinical Practice. *Circulation: Cardiovascular Interventions*. 2016;9(9):3940. [[CrossRef](#)]
10. Roffi M, Kulcsár Z, Carrera E, Cremonesi A. Carotid artery stenting. *Heart*. 2016;102(13):1059-69. [[CrossRef](#)] [[PubMed](#)]
11. de Donato G, Setacci C, Umemoto T, Reimers B. Commentary: Inside of the Interaction Between the Plaque and the Stent Optical Coherence Tomography During Carotid Artery Stenting. *Journal of Endovascular Therapy*. 2015;22(6):950-1. [[CrossRef](#)] [[PubMed](#)]
12. Cremonesi A, Castriota F, Secco GG, Macdonald S, Roffi M. Carotid artery stenting: an update. *European heart journal*. 2015;36(1):13-21. [[CrossRef](#)] [[PubMed](#)]
13. Shayan M, Chun Y. An overview of thin film nitinol endovascular devices. *Acta biomaterialia*. 2015;21:20-34. [[CrossRef](#)] [[PubMed](#)]
14. Sadideen H, Taylor PR, Padayachee TS. Restenosis after carotid endarterectomy. *International journal of clinical practice*. 2006;60(12):1625-30. [[CrossRef](#)] [[PubMed](#)]
15. Chun Y, Levi D, Mohanchandra K, Fishbein M, Carman G. Novel micro-patterning processes for thin film NiTi vascular devices. *Smart Materials and Structures*. 2010;19(10):105021. [[CrossRef](#)]
16. Mohanchandra K, Ho KK, Carman GP. Electrical characterization of NiTi film on silicon substrate. *Journal of intelligent material systems and structures*. 2004;15(5):387-92. [[CrossRef](#)]
17. Krejza J, Arkuszewski M, Kasner SE, Weigle J, Ustymowicz A, Hurst RW, et al. Carotid artery diameter in men and women and the relation to body and neck size. *Stroke*. 2006;37(4):1103-5. [[CrossRef](#)] [[PubMed](#)]
18. Babiker MH, Gonzalez LF, Albuquerque F, Collins D, Elvikis A, Frakes DH. Quantitative effects of coil packing density on cerebral aneurysm fluid dynamics: an in vitro steady flow study. *Annals of biomedical engineering*. 2010;38(7):2293-301. [[CrossRef](#)] [[PubMed](#)]
19. Oktar S, Yücel C, Karaosmanoglu D, Akkan K, Ozdemir H, Tokgoz N, et al. Blood-flow volume quantification in internal carotid and vertebral arteries: comparison of 3 different ultrasound techniques with phase-contrast MR imaging. *American journal of neuroradiology*. 2006;27(2):363-9. [[PubMed](#)]
20. Hopf-Jensen S, Marques L, Preiß M, Müller-Hülsbeck S. Initial clinical experience with the micromesh Roadsaver carotid artery stent for the treatment of patients with symptomatic carotid artery disease. *Journal of Endovascular Therapy*. 2015;22(2):220-5. [[CrossRef](#)] [[PubMed](#)]

21. Bosiers M, Deloose K, Torsello G, Scheinert D, Maene L, Peeters P, et al. The CLEAR-ROAD study: evaluation of a new dual layer micromesh stent system for the carotid artery. *EuroIntervention: journal of EuroPCR in collaboration with the Working Group on Interventional Cardiology of the European Society of Cardiology*. 2015;12(1).
22. Nerla R, Castriota F, Micari A, Sbarzaglia P, Secco GG, Ruffino MA, et al. Carotid artery stenting with a new-generation double-mesh stent in three high-volume Italian centres: clinical results of a multidisciplinary approach. *EuroIntervention: journal of EuroPCR in collaboration with the Working Group on Interventional Cardiology of the European Society of Cardiology*. 2016;12(5):677. [[CrossRef](#)] [[PubMed](#)]
23. Kedev S, Petkoska D, Zafirovska B, Vasilev I, Bertrand OF. Safety of slender 5Fr transradial approach for carotid artery stenting with a novel nitinol double-layer micromesh stent. *The American journal of cardiology*. 2015;116(6):977-81. [[CrossRef](#)] [[PubMed](#)]
24. Kealey CP, Chun YJ, Viñuela FE, Mohanchandra KP, Carman GP, Vinuela F, et al. In vitro and in vivo testing of a novel, hyperelastic thin film nitinol flow diversion stent. *Journal of Biomedical Materials Research Part B: Applied Biomaterials*. 2012;100(3):718-25. [[CrossRef](#)] [[PubMed](#)]
25. Ding Y, Dai D, Kallmes DF, Schroeder D, Kealey CP, Gupta V, et al. Preclinical Testing of a Novel Thin Film Nitinol Flow-Diversion Stent in a Rabbit Elastase Aneurysm Model. *American Journal of Neuroradiology*. 2016;37(3):497-501. [[CrossRef](#)] [[PubMed](#)]
26. Rajagopal V, Rockson SG. Coronary restenosis: a review of mechanisms and management. *The American journal of medicine*. 2003;115(7):547-53. [[CrossRef](#)]
27. Scott NA. Restenosis following implantation of bare metal coronary stents: pathophysiology and pathways involved in the vascular response to injury. *Advanced drug delivery reviews*. 2006;58(3):358-76. [[CrossRef](#)] [[PubMed](#)]
28. Weintraub WS. The pathophysiology and burden of restenosis. *The American journal of cardiology*. 2007;100(5):3-9. [[CrossRef](#)] [[PubMed](#)]
29. Chan P. Review: Developments in restenosis. *Journal of Renin-Angiotensin-Aldosterone System*. 2002;3(3):145-9. [[CrossRef](#)] [[PubMed](#)]
30. Mason RG, Sharp D, Chuang HY, Mohammad SF. The endothelium: roles in thrombosis and hemostasis. *Archives of pathology & laboratory medicine*. 1977;101(2):61-4.
31. van Hinsbergh VWM, editor *Endothelium—role in regulation of coagulation and inflammation* 2012: Springer.
32. Biela SA, Su Y, Spatz JP, Kemkemer R. Different sensitivity of human endothelial cells, smooth muscle cells and fibroblasts to topography in the nano–micro range. *Acta Biomaterialia*. 2009;5(7):2460-6. [[CrossRef](#)] [[PubMed](#)]
33. Vandrangi P, Gott SC, Kozaka R, Rodgers VGJ, Rao MP. Comparative endothelial cell response on topographically patterned titanium and silicon substrates with micrometer to sub-micrometer feature sizes. *PloS one*. 2014;9(10):111465. [[CrossRef](#)] [[PubMed](#)]
34. Aubin H, Nichol JW, Hutson CB, Bae H, Sieminski AL, Cropek DM, et al. Directed 3D cell alignment and elongation in microengineered hydrogels. *Biomaterials*. 2010;31(27):6941-51. [[CrossRef](#)] [[PubMed](#)]
35. Shen Y, Wang G, Chen L, Li H, Yu P, Bai M, et al. Investigation of surface endothelialization on biomedical nitinol (NiTi) alloy: Effects of surface micropatterning combined with plasma nanocoatings. *Acta biomaterialia*. 2009;5(9):3593-604. [[CrossRef](#)] [[PubMed](#)]

36. Belkaid W, Thostrup P, Yam PT, Juzwik CA, Ruthazer ES, Dhaunchak AS, et al. Cellular response to micropatterned growth promoting and inhibitory substrates. *BMC biotechnology*. 2013;13(1):86. [\[CrossRef\]](#) [\[PubMed\]](#)
37. Vartanian KB, Kirkpatrick SJ, Hanson SR, Hinds MT. Endothelial cell cytoskeletal alignment independent of fluid shear stress on micropatterned surfaces. *Biochemical and biophysical research communications*. 2008;371(4):787-92. [\[CrossRef\]](#) [\[PubMed\]](#)
38. Dike LE, Chen CS, Mrksich M, Tien J, Whitesides GM, Ingber DE. Geometric control of switching between growth, apoptosis, and differentiation during angiogenesis using micropatterned substrates. *In Vitro Cellular & Developmental Biology-Animal*. 1999;35(8):441-8. [\[CrossRef\]](#) [\[PubMed\]](#)



© 2016 by the authors; licensee *Preprints*, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons by Attribution (CC-BY) license (<http://creativecommons.org/licenses/by/4.0/>).