

Article

Development of a MEMS Sensor System for *In-Situ* Monitoring of the Engineered Barrier in a Geological Disposal Facility

Wenbin Yang, Rebecca J Lunn *, Alessandro Tarantino and Gráinne El Mountassir

Department of Civil and Environmental Engineering, University of Strathclyde, Glasgow G1 1XJ

* Correspondence: Rebecca.lunn@strath.ac.uk; Tel.: +44-141-548-2826

Abstract: Geological disposal facilities for radioactive waste pose significant challenges for robust monitoring of environmental conditions within the engineered barriers that surround the waste canister. Temperatures are elevated, due to the presence of heat generating waste, relative humidity varies from 20% to 100%, and swelling pressures within the bentonite barrier can typically be 2-10 MPa. Here, we test the robustness of a bespoke design MEMS sensor-based monitoring system, which we encapsulate in polyurethane resin. We place the sensor within an oedometer cell and show that despite a rise in swelling pressure to 2 MPa, our relative humidity (RH) measurements are unaffected. We then test the sensing system against a traditional RH sensor, using saturated bentonite with a range of RH values between 50% and 100%. Measurements differ, on average, by 2.87% RH, and a particularly far apart for high values of RH. However, bespoke calibration of the MEMS sensing system using saturated solutions of known RH, reduces the measurement difference to an average of 1.97% RH, greatly increasing the accuracy for RH values close to 100%.

Keywords: monitoring; geological disposal; sensor; relative humidity; bentonite; engineered barrier system; MEMS; geological disposal

1. Introduction

Real-time monitoring of deep geological disposal facilities (GDFs) for radioactive waste disposal is a significant challenge. The operational timescales of a GDF mean that monitoring technologies must function reliably over timescales in excess of 100 years [1]. A regulatory requirement of any GDF is likely to be the *in-situ* monitoring of the thermo-hydro-mechanical-chemical (THMC) behaviour of the engineered barrier system (EBS) that surrounds the waste canister. Monitoring creates significant challenges, temperatures can be highly elevated due to the presence of heat generating waste, relative humidity (RH) varies from 20% to 100%, and swelling pressures within the bentonite barrier are typically in excess of 2 MPa.

Most geological disposal concepts, for example the Swedish KBS-3V concept, are based on an EBS composed of a compacted bentonite buffer, which surrounds the waste canister (e.g. Figure 1). Post deposition, the bentonite buffer saturates via groundwater ingress from the surrounding rock, which results in a swelling pressure of between 2 and 10 MPa to ensure hydraulic sealing between the EBS, the surrounding rock and the central waste canister. Further, the very low hydraulic permeability of the bentonite ensures that, should canister failure occur, radionuclide transport would be extremely slow, since it is via diffusion only. Finally, the plastic nature of the saturated bentonite within the EBS also protects the canister from structural damage during small earthquakes [2].

Historically, an extensive range of relative humidity sensors have been deployed in radioactive waste disposal facilities and in underground testing laboratories over the past decades [3, 4]. While the measurement principle of the sensors varies, one common restraint of these traditional sensors lies in the unit size of the sensor (typically in the order of 10 cm), which limits the spatial resolution of the sensing device.

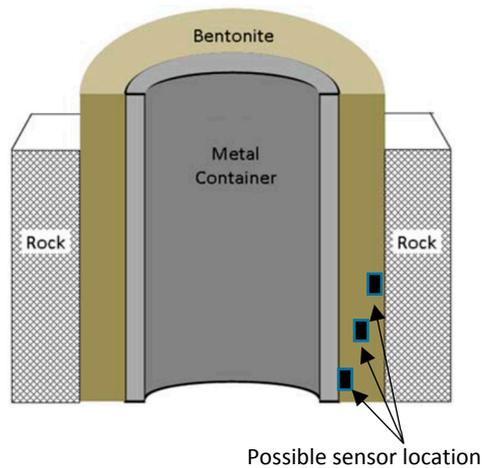


Figure 1. Schematic cross-section through the bentonite engineered barrier system

This research focuses on testing of a MEMS-based (Micro-Electro-Mechanical System) sensing system, developed in [5] for monitoring relative humidity within, or adjacent to, the compacted bentonite buffer in the EBS. Application of MEMS sensors in GDFs and other civil engineering projects still faces several key challenges in the engineering field [6]. This paper extends our previous research [5] by testing the performance of bespoke encapsulated MEMS sensors within saturated bentonite under swelling pressures of 2MPa. We show that our encapsulated MEMS monitoring system can withstand swelling pressures in excess of 2MPa and that, through improved sensor calibration, accurate measurements of compacted bentonite relative humidity can be achieved even up to RH values of 100%.

2. Materials and Methods

MEMS sensors provide higher measurement accuracy, improved spatial resolution in a limited space, and a longer life cycle resulting from low power consumption in the order of microwatts [7]. A first prototype of a multi-sensor monitoring system was presented in [5]. The system contains the Maxim® 31725 temperature sensor [8] and the Sensirion® SHT25 relative humidity sensor [9]. The Maxim® 31725 temperature sensor has a typical precision of $\pm 0.5^{\circ}\text{C}$ for a measurement range between -55°C and 150°C , and the Sensirion® SHT25 RH sensor has a labelled precision level of $\pm 1.8\%$ within the 10%-90% RH range, and $\pm 3\%$ for the full RH range. Both sensors have a chip dimension of 3mm x 3mm x 1mm, and are integrated onto a single printed circuit board (Figure 2). To minimise size, the sensor block 9mm x 11mm, is limited to hosting the sensor and its connector, all other functional components are integrated onto the motherboard that can be installed outside the bentonite barrier. The power supply and signal transmission are maintained by heat-resistant PTFE-coated wires that are compatible with temperatures between -60°C and 200°C . In future, these wires are planned for replacement by a wireless transmission system, which eliminates wire installation concerns, although at the expense of slightly increased sensor size.

To avoid direct contact between the sensor and the bentonite, a PTFE filter membrane cap designed by Sensirion® [10] was incorporated to cover the RH sensor on the PCB board prior to encapsulation. The filter protects the sensor from mechanical impact and contamination and prevents liquid water entering the sensors by capillarity, thus invalidating the measurement. At the same time, it allows the propagation of water vapour molecules between the measuring environment and the RH sensor. The sensor was then encapsulated via a 'potting' method [11] that uses polyurethane resin as an encapsulation material. This resulted in a rectangular polyurethane block that enclosed the sensor, with window for the measurement of RH (Figure 2). The encapsulated sensor block has similar dimensions to the sensor board prior to encapsulation, thus maintaining the small size. Since the MEMS temperature sensor is entirely encompassed during polyurethane encapsulation, it is unaffected by the bentonite, so is not discussed further. By contrast, the RH humidity sensor relies

on detection through the sensing window (Figure 2) and its accuracy may be compromised either by contact via liquid phase with the pore-water of the saturated bentonite, or by the swelling pressure that is exerted.

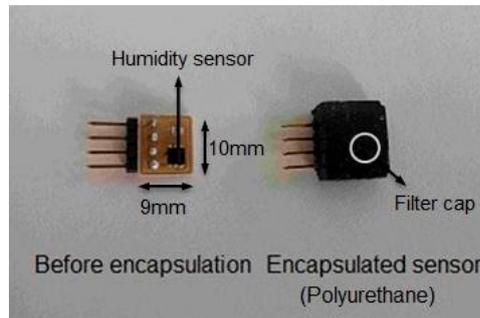


Figure 1. SHT25 sensor board before and after encapsulation

Experiment 1 focuses on verifying the mechanical robustness of the RH sensor under the swelling pressure exerted by hydrated bentonite. The test was carried out in an engineered oedometer cell, specifically designed by the Universitat Politècnica de Catalunya, as shown in Figure 3. The oedometer cell is separated into two sections by a ceramic-disc-supported thin membrane. On top of the membrane is an enclosed water reservoir connected to the GDS pressure volume controller, which controls the water pressure inside the reservoir within the range 0 – 2 MPa and, hence, the total vertical stress applied to the sample. A compacted bentonite block was fitted in the cavity below the membrane. The compacted MX-80 bentonite was drilled to form a 20mm-thick cylinder block, with a diameter of 50mm. The size of the bentonite block corresponded exactly to the dimension of the cavity inside the oedometer cell, in order to ensure that the top surface of the bentonite block was in firm contact with the membrane.

Hydration of the bentonite occurred through injection of deionised water from channel A (Figure 4) onto the top surface of the bentonite. The gap between the bentonite block and the side ring of the oedometer was sealed by polyurethane resin, in order to inhibit the ingress of water down the sides of the bentonite so as to achieve uni-directional water flow from the top surface to the bottom surface of the bentonite block.

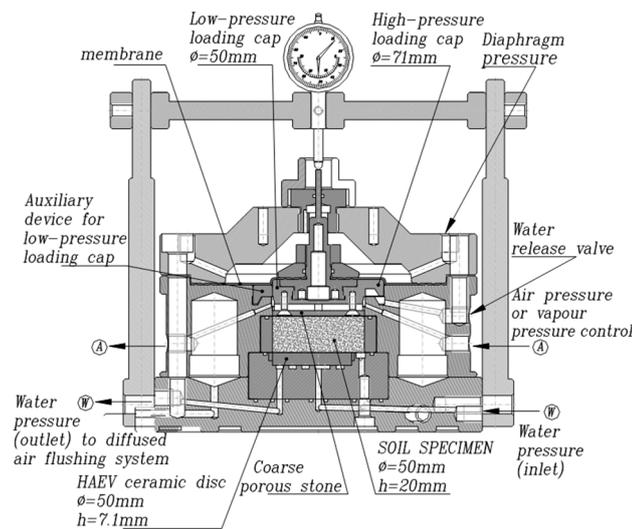


Figure 2. Cross-sectional structure of the oedometer cell.

In order to insert two sensors (side-by-side), a rectangular groove was carved into the base of the bentonite block, as shown in Figure 4. Two RH sensors were fitted into the groove, ensuring a firm contact with the bentonite block. This allowed the relative humidity at the bottom of the bentonite block to be measured during hydration. This installation minimised the volume of air between the sample and the sensor ensuring a rapid response time. The electrical wires connecting

the sensors to the control system were meticulously guided through channels beneath the cavity to the outside of the oedometer cell, and connected to the controller board. The exterior entrances to these channels were sealed via application of polyurethane, in order to block the air ventilation through the channel, and hence to prevent pore-water evaporation from the sample and, most of all, water vapour flow through any gap between the sample and the sensor towards the outside of the cell.



Figure 3. Placement of the RH sensors in the oedometer and the groove at the bottom of the bentonite.

The principal objective of the experiment was to test the mechanical robustness of the RH sensors embedded at the base of the bentonite block under increasing swelling pressure due to hydration of the bentonite block. In order to reach swelling pressures in the range of 2MPa, the bentonite block must be fully constrained in all directions. As a consequence, the position of the membrane on top of bentonite was kept stationary by continuously increasing the water pressure in the upper reservoir such that the applied pressure on the top of the sample was equal to the swelling pressure generated by the hydrating bentonite. A displacement gauge was placed on top of the oedometer cell to operate as a null sensor. When a displacement was recorded by the displacement gauge, the water pressure in the GDS was manually incremented in a step-wise fashion to restore zero vertical displacement. The increment of water pressure in the GDS was noted after each adjustment, alongside, the digitally recorded RH readings.

Experiment 2 was designed to test the accuracy of the sensing system within the saturated bentonite. There exist several different methods to measure the relative humidity of the water vapour in equilibrium with the bentonite blocks. Besides the installation of a traditional RH sensor at the point of interest (which would disturb the sample and be too large as to be incorporated), it is also possible to measure the RH using a Chilled-Mirror Psychrometer [12]. The psychrometer used in this experimental programme is a product of Decagon Devices, Inc. and is known as a WP4 Dew Point Potentiometer. Although the psychrometer actually measures the relative humidity RH, the data are displayed in terms of total suction Ψ according to the psychrometric law:

$$\Psi = -\frac{RT}{v_{w0}\omega_v} \ln\left(\frac{u_v}{u_{v0}}\right) = -\frac{RT}{v_{w0}\omega_v} \ln(RH), \quad (\text{Equation 5.1})$$

where R is the universal gas constant (8.31432Jmol⁻¹K⁻¹), T is the absolute temperature in Kelvin, v_{w0} is the specific volume of water, and ω_v is the molecular mass of water vapor (18.016g/mol). u_v and u_{v0} represent the partial pressure of water vapour and the vapour pressure of water vapour at saturation, respectively. For water vapour at 20°C, this equation can be simplified to:

$$\Psi = -135022\ln(RH), \quad (\text{Equation 5.2})$$

where Ψ is given in kPa. This equation was used to derive the relative humidity RH measured in the air surrounding the sample from the value of total suction Ψ displayed by the instrument.

By comparing the RH measured using a WP4 dewpoint potentiometer with the RH measured by the sensing system, within the same hydrated bentonite block, we can validate the *in-vivo* measurement accuracy of the RH sensor whilst embedded in a bentonite block.

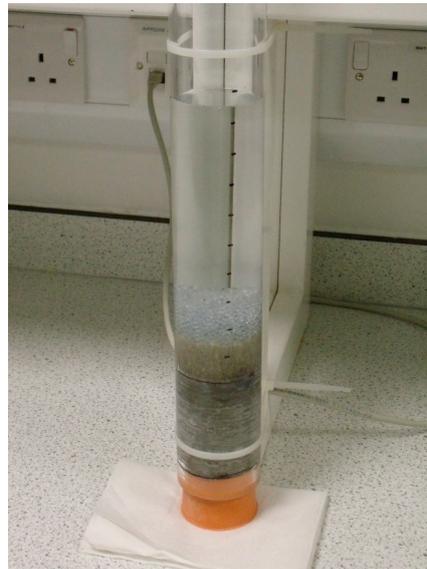


Figure 4. Hydration of bentonite block in polycarbonate tube.

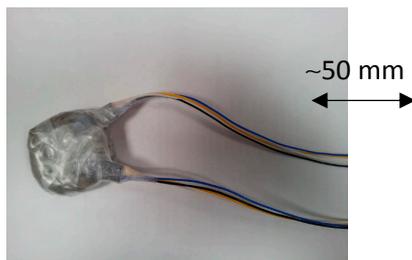


Figure 5 Hydrated bentonite block wrapped with RH sensors.

Experiment 2 was carried out using the following steps: an MX-80 bentonite block was first cut and drilled to form a short cylinder with a diameter of 5cm and a height of approximately 7.5cm. The bentonite cylinder was then sealed on the sides using an impermeable membrane and fixed to the bottom of a polycarbonate tube, as shown in Figure 5. The internal diameter of the tube was chosen to be the same as the diameter of the bentonite cylinder, with any remaining void space between the bentonite and the tube wall being filled by the membrane. Water was injected from the top of the tube and was only in contact with the upper surface of the bentonite block. Hence, the hydration of the bentonite block took place gradually from top to bottom, and a gradient of water content along the length of the bentonite cylinder was formed during this hydration process.

The duration of hydration process varied between tests with a minimum of 7 days and a maximum of 20 days. This was to achieve different water content levels in the bentonite samples such that sensor accuracy could be tested at a range of relative humidity values. The hydrated bentonite block was then removed from the tube and cut into slices approximately 2.5cm thick. Rectangular cavities were cut into both sides of each 2.5 cm bentonite block to install the RH sensors. The hydrated bentonite block and the sensors were then wrapped using an impermeable membrane to allow for water vapour equilibrium in the air surrounding the sample, as shown in Figure 6. The RH data was regularly measured by the sensing system over a period of several days until a constant RH was recorded, indicating that i) uniform distribution of suction was achieved within the bentonite block and ii) water vapour surrounding the bentonite block achieved equilibrium with suction in the bentonite. The bentonite block was then unsealed and a small sample of each block was

immediately put into the WP4. The RH of the sample could be calculated from the displayed value of total suction Ψ using equation 5.2.

3. Results

3.1. Mechanical Robustness of the Sensing System

The results of Experiment 1, the oedometer cell test, are plotted in Figure 7. Shown is the relative humidity measured by both RH sensors alongside the increase in total vertical stress (water pressure controlled by the GDS), in turn associated with the swelling pressure generated by the progressive hydration of the sample. A temporary signal loss occurred between days 4 and 5, caused by a bad contact on the sensor-to-wire connector under the influence of the increasing swelling pressure. The sensor itself, however, is fully functional during the entire experimental period of 26 days and remains unaffected by a swelling pressure of >2MPa, which was maintained for a 10-day period. It is worth noting that the swelling pressure and the RH recorded by the two sensors levels off at the same time, highlighting the coherence of the RH measurement.

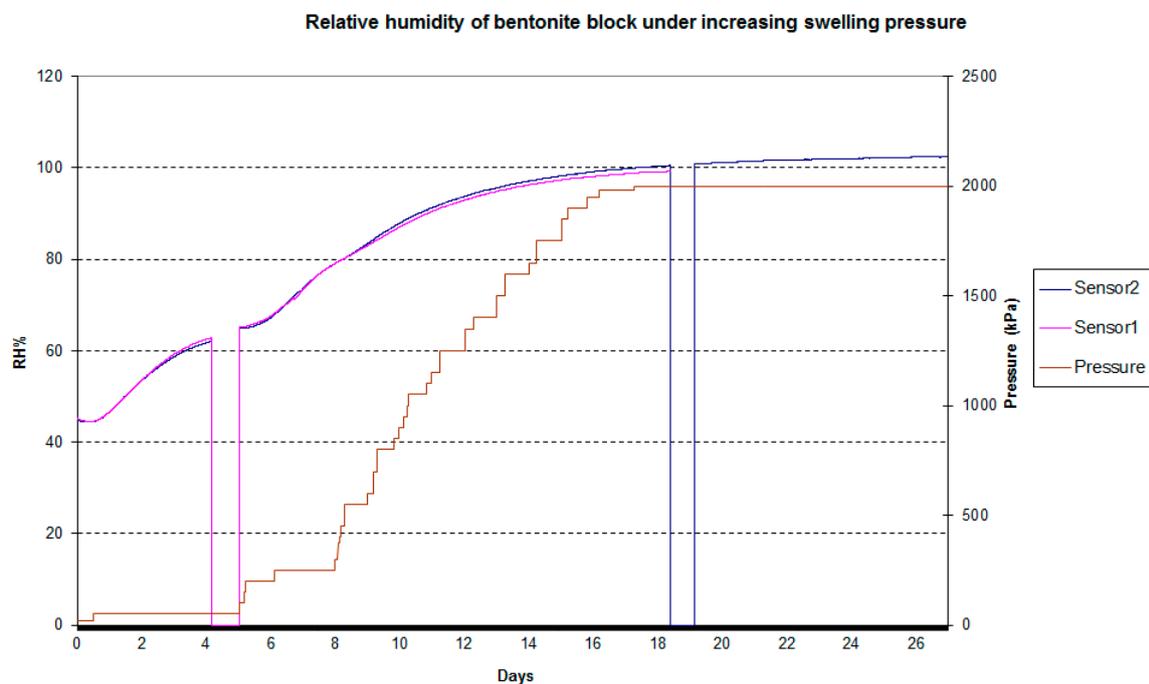


Figure 6 Evolution of relative humidity and GDS water pressure during the hydration of the bentonite within the oedometer cell

At the end of the experiment, both sensors were removed from the oedometer cell and tested again in the open air. Test results revealed that both sensors were fully functional after sustaining the high swelling pressure, without any deterioration in sensor accuracy. The swelling pressures tested here are at the lower end of those that would be experienced in a geological disposal facility, sensor performance was entirely unaffected and the sensors proved to be robust. The observed signal loss would be eliminated by more robust cable connection methods (these were soldered by hand) or by the incorporation of a wireless transmission onto the sensing system.

3.2. Sensor accuracy within the saturated bentonite

Table 1 shows the results for both measurement methods (WP4 and RH sensing system) for 7 samples, covering a range of RH levels from 52% to 100%. Analysis of the data in Table 1 shows that the RH measured by the two methods is generally coherent, but with a mean discrepancy of

2.87(%RH). With the exception of sample No. 1, sample differences are less than 4%. For sample No. 1, at very high humidity there is a discrepancy of 8.1%.

Table 1 RH of hydrated bentonite samples measured by psychrometer and by the sensor

Sample No.	Suction (MPa)	RH calculated from suction	RH measured by sensor	Difference
1	-0.09 MPa	99.9%	108.0%	-8.10%
2	-5.22 MPa	96.2%	97.8%	-1.60%
3	-9.47 MPa	93.3%	97.1%	-3.80%
4	-34.76 MPa	77.4%	76.8%	0.60%
5	-44.69 MPa	71.9%	73.1%	-1.20%
6	-83.55 MPa	54.1%	52.0%	2.10%
7	-96.94 MPa	49.0%	51.7%	-2.70%

4. Discussion

The differences noted between the measurements of the sensing system developed here and the RH derived using the WP4 psychrometric are liable to be due to error from two sources. The WP4 method tends to underestimate relative humidity for values of soil RH higher than the laboratory relative humidity. When the measurement chamber of the WP4 is open to insert the sample, ambient air at the laboratory RH invades the chamber. As the chamber is closed, evaporation then occurs from the sample into the air in the chamber until equilibrium is established. As a result, the water content of the sample and, hence, the relative humidity in equilibrium with the sample, decreases. This error was minimised by placing samples that were as large as possible into the WP4 chamber (i.e. a low surface to mass ratio).

Furthermore, similar to any other technique for relative humidity measurement, the WP4 tends to be inaccurate at very high relative humidity. When the RH is close to 100%, even very small fluctuations of temperature cause drop condensation in the measurement chamber that bias the measurement. However, among the different measurement techniques, the WP4 is perhaps the one that ensures the largest measurement range at high RH values (up to 99.0-99.5%). Other commercial RH sensors, including thermocouple and transistor psychrometers, are characterised by a shorter measurement range (up to 98.5-99.0%) [13].

For the case of the RH MEMS sensor tested in this experimental programme, another source of inaccuracy is the non-linearity of the relationship between the air relative humidity and the volumetric water content of the hygroscopic dielectric material placed between the two plates of the capacitive sensor. When relative humidity approaches 100%, the sensing element approaches saturation. As a result, variations in RH generate variations in volumetric water content of the dielectric material that tend to become smaller and smaller as saturation is approached. In turn, variations in capacitance and, hence, electrical signal, tend to become negligible. Since the derivative of the capacitance versus RH function tends to zero as saturation is approached, there is a loss of sensitivity of the instrument close to saturation.

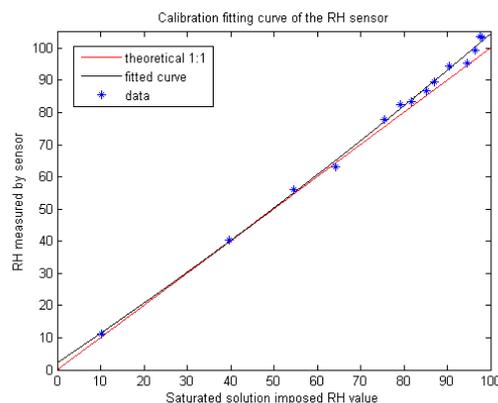


Figure 10 Fitting curve of the calibration model for the RH sensor

This loss in accuracy associated with the non-linearity of the calibration curve was quantified in [5] by the use of a variety of saturated chemical solutions, each of which had a different, known saturated relative humidity when placed within a sealed, temperature-controlled environment. Hence, these could be used as accurate reference points without the requirement for any type of sensor. The results of these experiments are reproduced in Figure 10. Data points lie on the 1:1 line (in red) in the low to medium RH range, but deviate consistently at high RH values. If the relative humidity values returned by the sensor RH are treated as raw sensor data, the sensor can be calibrated using the fitted curve in Figure 10. An adjusted estimate of the relative humidity RH_A can be from the calibration equation in Figure 10 is:

$$RH = 0.001204(RH_A)^2 + 0.9015RH_A + 2.182, \text{ (Equation 3)}$$

Solving this quadratic equation gives an adjusted value of the measured relative humidity based on the sensor calibration curve, RH_A . The adjusted values for relative humidity RH_A are shown in Table 2. The difference between the measured value (RH_A) and that derived from the WP4 data has now reduced. The mean of the differences between them is now 1.97% and the discrepancy between the two values for sample number 1, at high humidity, has dropped from 8.1% to 1.9%.

The results of both Experiment 1 and Experiment 2 described here, show that our MEMs-based sensing system is a promising miniaturised alternative to traditional RH sensors in geological disposal facilities. It is sufficiently robust to withstand at least 2MPa of swelling pressure and, once calibrated, is capable of accurate RH measurement over the wide range of RH values (20% - 100%) encountered within an EBS.

Table 2 Corrected RH of hydrated bentonite samples measured by psychrometer and by the sensor

Sample No.	RH calculated from suction	RH_A corrected	Difference
1	99.9%	101.8%	-1.90%
2	96.2%	93.1%	3.10%
3	93.3%	92.6%	0.70%
4	77.4%	74.7%	2.70%
5	71.9%	71.3%	0.60%
6	54.1%	51.6%	2.50%
7	49.0%	51.3%	-2.30%

Acknowledgments: This research has been supported by EPSRC consortium grant EP/I036427/1 'SAFE Barriers – a Systems Approach For Engineered Barriers' (2012-2016). This was co-funded by EPSRC and Nuclear Decommissioning Authority Radioactive Waste Management Directive, now Radioactive Waste Management".

References

1. Lidskog, R. and Andersson, A.C. (2002) The Management of Radioactive Waste: A Description of Ten Countries. SKB report, ISBN 91-973987-3-X.
2. Juvankoski, M., Ikonen, K., and Jalonen, T. (2012) Buffer production line 2012: Design, production and initial state of the buffer. Posiva report 2012-17.
3. Alonso, E.E., Springman, S.M. and Ng, W.W. (2009) Monitoring large-scale tests for nuclear waste disposal. *Geotechnical and Geological Engineering*, 26, 817–826.
4. Breen, B.J., Garcia-Sineriz, J.L., Maurer, H., Mayer, S., Schröder, T.J. and Verstricht, J. (2012) EC MoDeRn Project: In-situ demonstration of innovative monitoring technologies for geological disposal. WM2012 Conference. Available at www.wmsym.org/archives/2012/papers/12053.pdf
5. Yang W., Lunn R.J. and Tarantino A. (2015) MEMS sensor-based monitoring system for engineered geological disposal facilities. *Mineralogical Magazine*. Vol. 79(6): 1475–1483.
6. Ceylan H., Gopalakrishnan, K., Taylor, P., Shrotriya, P., Kim, S., Prokudin, M., Wang, S., Buss, A.F., Zhang, J. et al. (2011) A Feasibility Study on Embedded Micro-electromechanical Sensors and Systems (MEMS) for Monitoring Highway Structures. Iowa Highway Research Board Report No. TR-575.
7. Akyildiz, I.F., Su, W., Sankarasubramanian, Y. and Cayirci, E. (2002) Wireless sensor networks: a survey. *Computer Networks*, 38, 393–422.
8. Maxim® 31725 datasheet. Ver.2013. Available from: <http://datasheets.maximintegrated.com/en/ds/MAX31725-MAX31726.pdf>
9. Sensirion® SHT25 datasheet. Ver.2014. Available from: http://www.sensirion.com/fileadmin/user_upload/customers/sensirion/Dokumente/Humidity/Sensirion_Humidity_SHT25_Datasheet_V3.pdf
10. Sensirion® Filter Cap SF2 datasheet. Ver.2011. Available from:
11. Chao, N. H., Dispenza, J. A. and DeAngelis, M. E. (2012) Encapsulating protective layers for enhancing survivability of circuit board assemblies in harsh and extreme environments, *ASME 2012 International Mechanical Engineering Congress and Exposition*, 9, 363-373
12. Bulut, R., Leong, E.C. (2008). Indirect measurement of suction. *Geotechnical and Geological Engineering*, 26(6): 21-32.