

Supporting information

A methodologic approach for the selection of bio-resorbable polymers in the development of medical devices: the case of poly(L-lactide-co- ϵ -caprolactone)

Alberto Cingolani ^{1,2}, Tommaso Casalini ^{1,3}, Stefano Caimi ¹, Antoine Klaue ¹, Mattia Sponchioni ⁴, Filippo Rossi ^{4,*} and Giuseppe Perale ^{1,3,*}


¹ Institute for Chemical and Bioengineering, Department of Chemistry and Applied Bioscience ETH Zurich, Vladimir-Prelog-Weg 1-5/10, 8093 Zürich, Switzerland; A.C. alberto.cingolani@chem.ethz.ch; T.C. tommaso.casalini@chem.ethz.ch; S.C. stefano.caimi@chem.ethz.ch; A.K. antoine.klaue@chem.ethz.ch.

² Industrie Biomediche Insubri SA (IBI), Via Cantonale 67, 6805 Mezzovico-Vira, Switzerland


³ Biomaterials Laboratory, Institute for Mechanical Engineering and Materials Technology, SUPSI – University of Applied Sciences and Arts of Southern Switzerland. Via Cantonale 2C, Galleria 2, 6928 Manno, Switzerland; G.P. giuseppe.perale@supsi.ch;

⁴ Department of Chemistry, Materials and Chemical Engineering “G. Natta”, Politecnico di Milano, 20100 Milan, Italy; M.S. mattia.sponchioni@polimi.it; F.R. filippo.rossi@polimi.it.

- Correspondence: filippo.rossi@polimi.it; Tel: +39 02-2399-3145
giuseppe.perale@supsi.ch; Tel.: +41-58-666-66-41

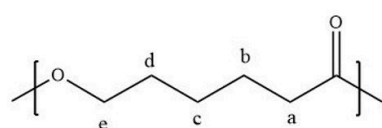

PCL unit



PLA unit


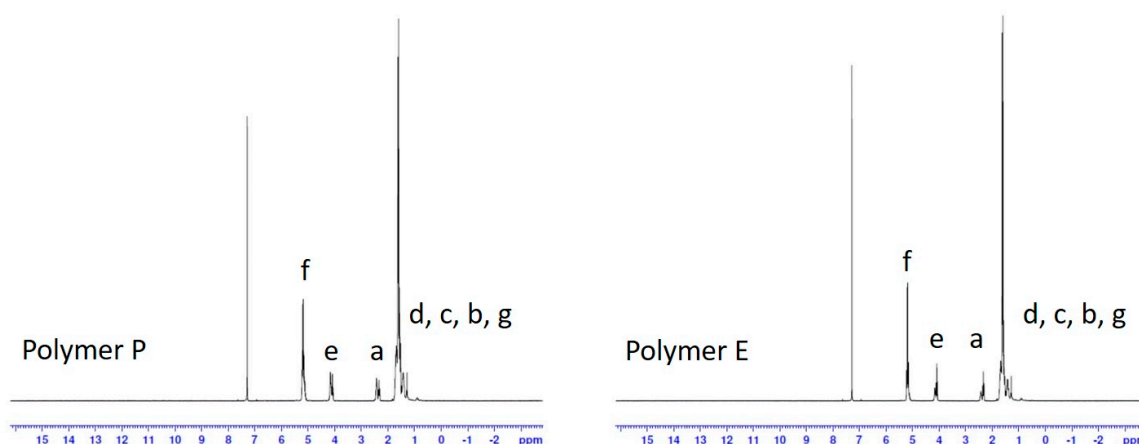


Figure S1. NMR spectra of P and E samples.

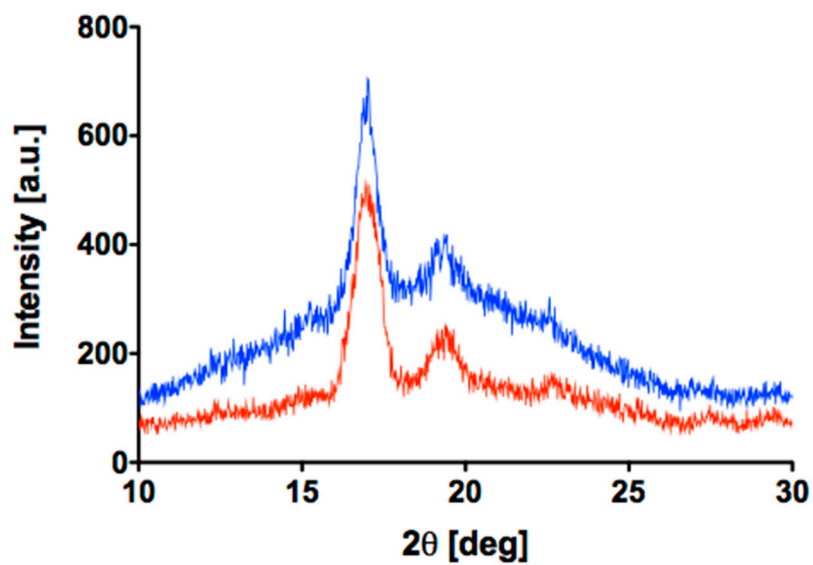


27

28

29

Figure S2. XRD spectra of P (blue line) and E (red line).

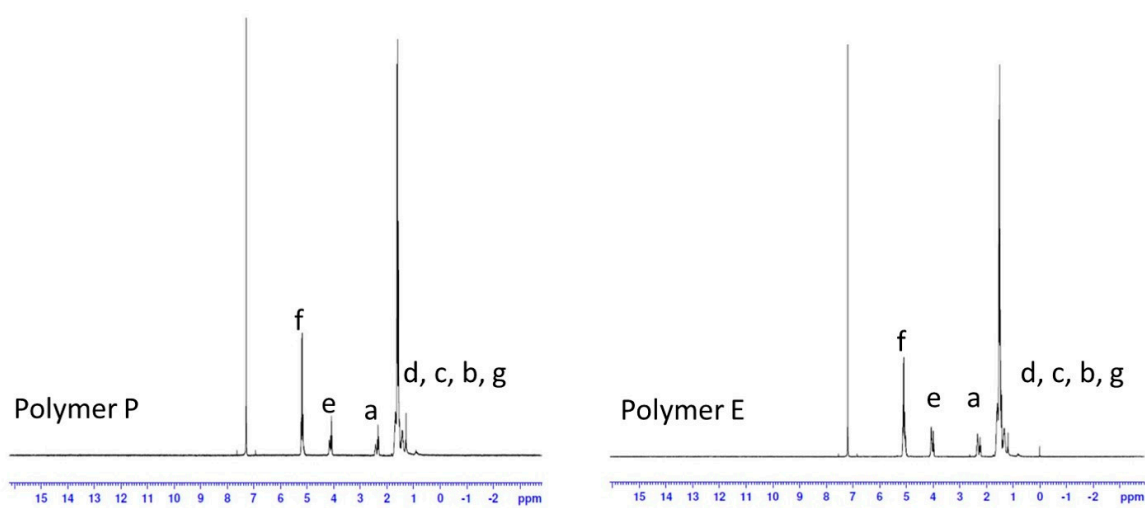


30

31

32

Figure S3. NMR spectra of P and E after EtO.

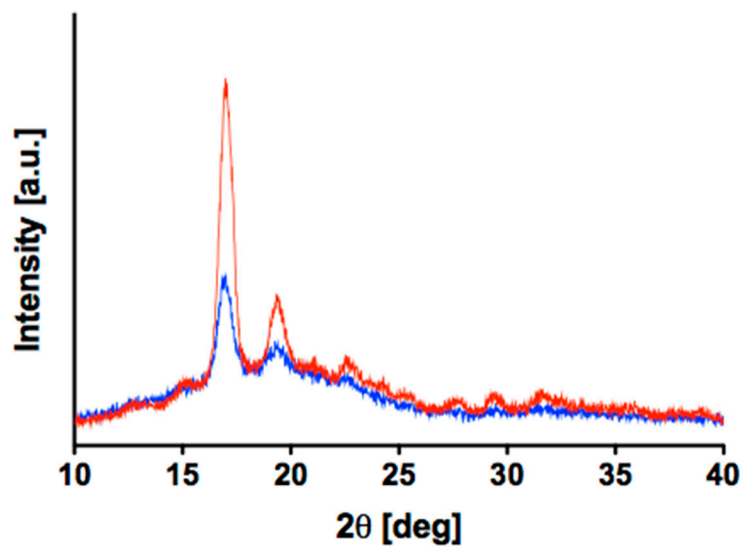


33

34

Figure S4. XRD spectra of P (blue line) and E (red line) after EtO.


35

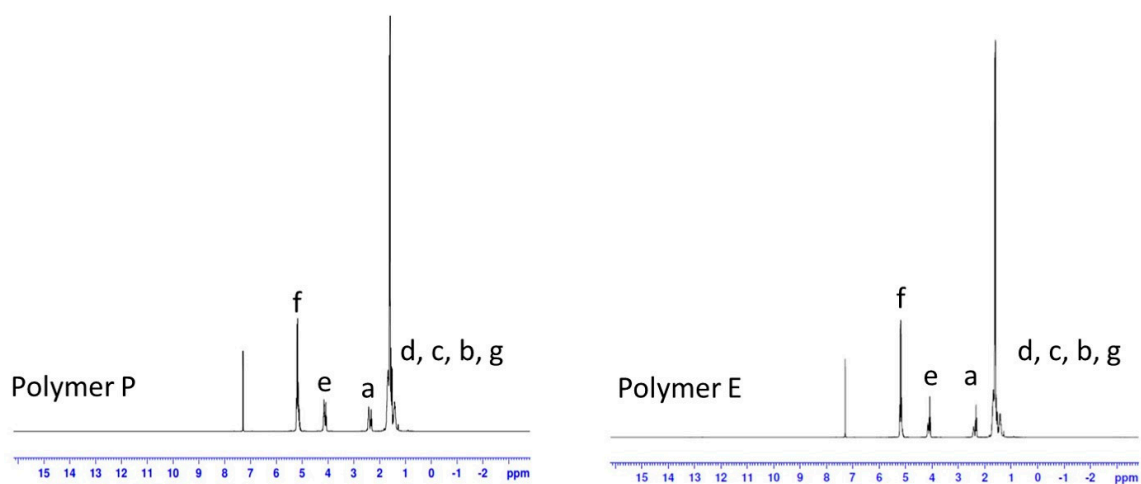

36

37

Figure S5. NMR spectra of P and E after electron beam irradiation.

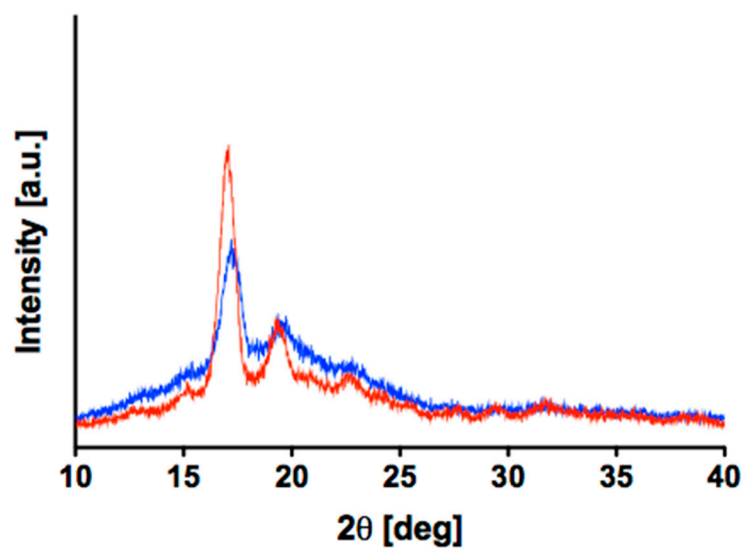

38

39

Figure S6. XRD spectra of P and E after electron beam irradiation.