


A Polymer-Gel Eye-Phantom for 3D Fluorescent Imaging of Millimetre Radiation Beams

Leonard H. Luthjens, Tiantian Yao and John M. Warman*


Delft University of Technology, Faculty of Applied Sciences, Department of Radiation Science and Technology, Section Radiation and Isotopes for Health, Mekelweg 15, 2629 JB DELFT, The Netherlands

*corresponding author: E-mail J.M.Warman@TUDelft.nl

Abstract: We have filled a 24 mm diameter glass sphere with a transparent polymer-gel that is radio-fluorogenic, i.e. it becomes (permanently) fluorescent when irradiated, with an intensity proportional to the local dose deposited. The gel consists of >99.9% tertiary-butyl acrylate (TBA) pre-polymerized to ~15% conversion, and ~100 ppm maleimido-pyrene (MPy). Its dimensions and physical properties are close to those of the vitreous body of the human eye. We have irradiated the gel with a 3 mm diameter, 200 kVp X-ray beam with a dose rate of ~1 Gy/min. A 3D (video) view of the beam within the gel has been constructed from tomographic images obtained by scanning the sample through a thin sheet of UV light. To minimize optical artifacts, the cell was immersed in a square tank containing a refractive-index-matching medium. The 20%-80% penumbra of the beam was determined to be ~0.4 mm. The research was a preparatory investigation of the possibility of using the method to monitor the millimetre diameter proton pencil beams used in ocular radiotherapy.

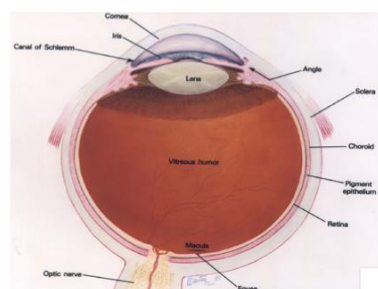

Anatomy of the eye
from NIH: National Eye Institute



Eye phantom with fluorescent image
of 3 mm diameter x-ray beam

Graphic abstract

Keywords: Radiotherapy eye-phantom; radio-fluorogenic gel; x-ray beam imaging; 3D radiation imaging; polymer gel dosimetry.

1. Introduction

The treatment of ocular tumours is fraught with difficulties due to the proximity of important healthy tissues involved in sight and/or brain function. Radiotherapy has been an important method of treatment using either brachytherapy or external beam procedures [1-4]. The small dimension of the organ makes the use of highly collimated beams of millimetre dimensions imperative. With the recent proliferation of clinical proton beam sources [5], the incorporation of proton pencil beams in cancer protocols has become a worldwide reality [6-8]. Because of this there is a current need for a medium capable of providing three-dimensional images with sub-millimeter spatial resolution of dose deposition in phantoms for confirmation of computer derived treatment protocols, equipment functioning, and for training clinical personnel [9].

A variety of methods involving 3D matrixes of one- and two-dimensional individual detectors are commercially available and presently used in the clinic. They are however incapable of achieving the sub-millimeter spatial resolution required for small beam applications. For this, molecular media that undergo a measureable physico-chemical change on a microscopic scale when irradiated are required. Since the first suggestion in 1950 by Day and Stein [10] of using a quasi-rigid, gel medium, several methods based on this basic formula have been developed and reviewed [11-17]. Unfortunately none have become generally accepted in the radiotherapy clinic [18-20]. The reasons for this lack of adoption can be ascribed to a combination of: the complexity of the gel formulations, often involving up to 5 components, and the corresponding difficulty of universal reproducibility; the lack of off-the-shelf availability compared with gaseous (IC) or solid-state devices; the delay in post-irradiation data analysis; and possibly the cost.

In this report we show how a radio-fluorogenic (RFG) polymer-gel [21, 22] can be used to provide a 3D image of the track of a narrow (3 mm diameter) X-ray beam in a volume as small as the human eye. An RFG gel is a two-component mixture whose components are commercially available, inexpensive and whose composition can be accurately determined by optical spectroscopy. The gel, which is tissue equivalent, becomes *permanently* fluorescent on irradiation with intensity proportional to the local dose deposited. The fluorescence can be tomographically scanned on-site immediately after irradiation and processed within minutes to yield 3D images of the radiation field [23]. The work reported here is a pilot study investigating the feasibility of applying RFG gel phantoms to the control of radiotherapy protocols and equipment for proton pencil beam treatment of eye tumours. It was driven by the recent construction of a proton radiotherapy clinic within the grounds of the authors' institute. The capability of making 2D, *bulk* images of proton pencil beams in an RFG gel was demonstrated previously by one of the authors using a high-energy physics particle accelerator [24].

2. Materials and Methods

2.1. RFG gel formation

The gel container used is a spherical borosilicate glass bulb 24 mm in outer diameter with a wall thickness of 1.7 mm; similar dimensions to those of the adult human eye. The bulb contains 5 mL of a transparent radiofluorogenic (RFG) gel with a gravimetric density of 0.91 kgL^{-1} and an electron density of $3.00 \times 10^{26} \text{ L}^{-1}$; values

that are close to the 1.01 kgL^{-1} and $3.35 \times 10^{26} \text{ L}^{-1}$ of the vitreous body of the eye, and the 1.18 kgL^{-1} and $3.84 \times 10^{26} \text{ L}^{-1}$ of chemically-related PMMA (often denoted "solid water"). The RFG gel consists of 15% pre-polymerised, inhibitor-free, tertiary-butyl acrylate (TBA; Sigma Aldrich purum #01775) to which is added approximately 100 ppm of the fluorogenic compound maleimido-pyrene (MPy; Sigma Aldrich P7908).

The RFG gel preparation procedure has been described in full previously [21, 22]. Briefly, the gel is preformed in the cell by ^{60}Co γ -irradiation ($\sim 15 \text{ Gy}$ at $\sim 1 \text{ Gy/min}$) of pure, de-aerated, inhibitor-free TBA to $\sim 15\%$ monomer conversion. Excess monomer is then pumped off leaving the polymer network deposited on the cell wall, as shown in Figure 1. The gel is reformed by adding a dilute solution of MPy in TBA equal to the volume of monomer pumped off and allowing time (~ 2 weeks) for reformation of the gel.

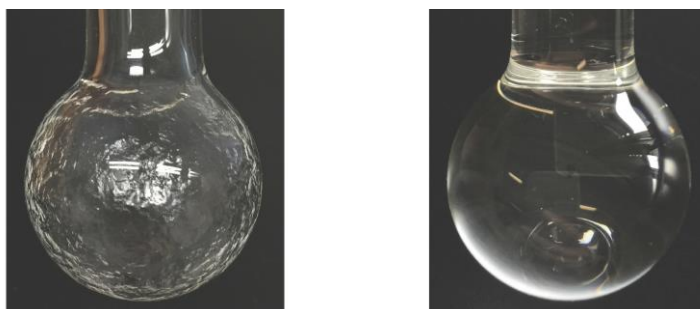


Figure 1. Left: The "eye-phantom" cell after radiation-induced polymerization of TBA to $\sim 15\%$ conversion and pumping-off the residual monomer leaving the polymer network. Right: The clear gel (re)formed on addition of a dilute solution of MPy in TBA and swelling of the polymer network.

2.2. X-ray Beam Irradiation

The gel, contained in the eye-phantom cell, was irradiated with 200 kVp X-rays from a Philips MCN 321 X-ray tube. The conical beam was restricted by a brass collimator with a circular channel 3.0 mm in diameter and 30 mm long inserted in a $120 \times 120 \text{ mm}^2$ square, 27 mm thick Al/Pb/Al attenuator. The dose rate at the exit of the collimator, 460 mm from the source target, was $\sim 1.0 \text{ Gy/min}$ for a beam current of 15 mA. The cell was irradiated for 20 minutes resulting in a total incident dose of $\sim 20 \text{ Gy}$. The basic irradiation set-up with optical rail, collimator and outline laser has been shown in a previous publication [23].

MD-V3 Gafchromic film (Lot Nr 02101602) was used as a secondary, 2D dosimeter for monitoring the incident and exit beam dose rates and cross-sections. The dose sensitivity of the film was calibrated against an X-ray Exposure Meter (Vinten Instruments) that was routinely calibrated at the Netherlands Metrology Institute. The derivation of the dose from the measured intensity reflected by the scanned films has been described in full in reference [25]. The film was attached to the front and rear faces of a 24 mm square borosilicate glass cell placed at the same position as the 24 mm diameter eye-phantom cell. These control measurements were made with the square cell containing either air or an identical gel to that used in the eye-phantom.

2.3. Fluorescence Imaging

Fluorescence imaging was carried out using the UV slit scanning method previously reported [23]. This yields a series of tomographic images that can be used to generate a 3D image of the fluorescence within the gel. The sheet of UV light at 385 nm was 2 mm thick and the cell was transported in 1 mm steps through the sheet for a total distance of 30 mm. The cell was immersed in a glycerol bath contained in a 40x40 mm² square borosilicate glass container with optically flat sides. This resulted in close matching of the refractive indexes of the surroundings (glycerol $n=1.47$) with that of the borosilicate glass cell walls ($n=1.47$) and the gel ($n=1.42$). This diminished optical artifacts caused by lensing and reflections at dielectric interfaces.

3. Results and Discussion

3.1. Test measurement with a standard fluorescent solution

In Figure 2 we show an image taken of a cell containing a micromolar concentration of the fluorescence-standard diphenyl anthracene (DPA) in cyclohexane. The image was taken with the UV excitation sheet positioned at the centre of the cell.

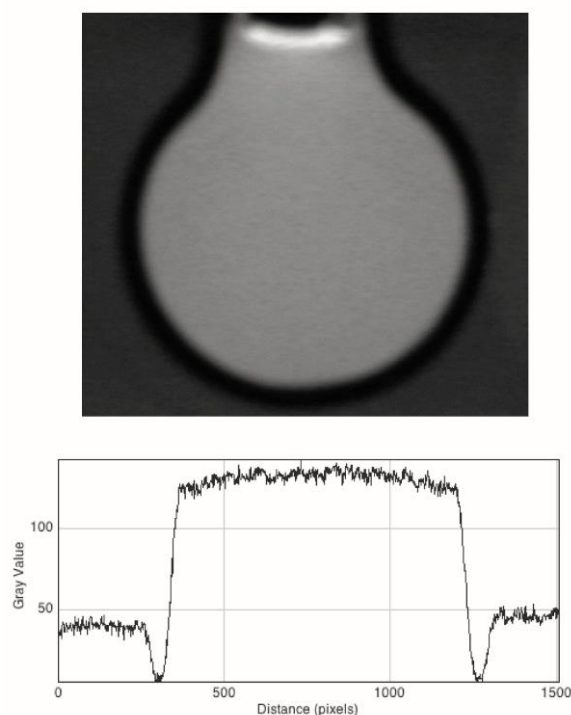


Figure 2. The fluorescence of a dilute solution of the fluorescence-standard diphenyl anthracene in the "eye-phantom" cell. The black "shadow" surrounding the cell, and corresponding intensity dips in the lower pixel profile, result from the non-fluorescent glass wall of the cell surrounded by the slightly fluorescent glycerol dielectric-matching bath.

The pixel profile shown in Figure 2 displays a close to uniform fluorescence within the volume of the cell. The slight (~8%) upward curvature is probably caused by a lensing effect due to the difference in refractive index between cyclohexane and glass (1.43 versus 1.47). The black "shadow" surrounding the liquid is due to the non-fluorescent glass cell wall. The slight increase in fluorescence outside the glass wall results from the fact that, in this measurement, the sample of glycerol used contained a fluorescent impurity. The presence of the impurity in the glycerol had a positive side to it since it allowed us to determine the number of pixels per mm in the images from the accurately measureable outer diameter of the cell of 24.0 mm. The value determined was 44 pixels per mm or 0.023 mm per pixel. This represents the ultimate practical limit to the spatial resolution of the measurements in the x/y plane. The thickness of the cell wall and the diameter of the gel could also be accurately determined from the scan in Figure 2 to be 1.7 mm and 20.6 mm respectively.

3.2. Radiochromic film measurements

An MD-V3 radiochromic film image of the X-ray beam incident on the cell is shown in Figure 3. As can be seen the beam was slightly oval with a long axis 14% larger than the short axis. This phenomenon is attributed to the fact that the 3.0 mm (perfectly) circular collimator is smaller than the 4 mm dimension of the tungsten target of the source resulting in partial "pinhole imaging" of the X-ray emission from the target.

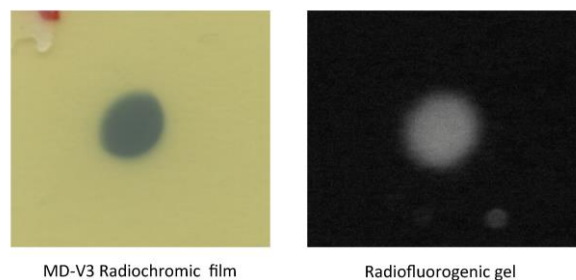


Figure 3. Left: The cross-sectional beam geometry as recorded using MD-V3 radiochromic film at the front face of the cell. Right: The fluorescent image as recorded in the RFG gel looking along the propagation (z) axis of the beam.

From a pixel profile line scan across the RC beam image in Figure 3 the 20-80% penumbra of the beam was found to be 0.41 mm and 0.54 mm for the incident and exit beams respectively. The spatial resolution of the film images is 300 dpi or 0.085 mm/pixel. The much larger penumbra value is therefore attributed to edge-dispersion in the intensity of the x-ray beam.

The central optical absorption in the profile scan was used together with relationship (2) to determine the incident and exit dose rates. For a cell containing air the values were 0.94 and 0.67 Gy/min; a decrease by 0.713. For a cell containing an RFG gel the values were 0.89 and 0.47 Gy/min; a decrease by 0.528. The decrease in dose rate between the incident and exit films is due to the conical expansion of the beam from z_1 (47.6 cm) to z_2 (50.0 cm) and to photon attenuation in the intervening media,

$$D'(z_2)/D'(z_1) = (z_1/z_2)^2 \exp\{-2[M\rho\delta]_{\text{glass}} + [M\rho\delta]_{\text{gel}}\} \quad (3)$$

In (3) M , ρ and δ are the mass attenuation coefficient, the gravimetric density and the length of the attenuating medium respectively. For the air-containing cell the attenuation by the cell contents is negligible and the overall decrease by a factor of 0.71 leads to a value of $2[M\rho\delta]_{\text{glass}} = 0.244$. Taking a borosilicate glass density of 2.3 g/cm^3 and a wall thickness of 0.17 cm results in a mass attenuation coefficient for the cell wall of $0.312 \text{ cm}^2/\text{g}$. From the dose rate decrease for the gel-containing cell we determine a value for $(2[M\rho\delta]_{\text{glass}} + [M\rho\delta]_{\text{gel}})$ of 0.540 or $[M\rho\delta]_{\text{gel}} = 0.296$ after subtracting the glass wall contribution determined above. Taking for the gel $\delta = 2.0 \text{ cm}$ and $\rho = 0.91 \text{ g/cm}^3$ results in $M_{\text{gel}} = 0.163 \text{ cm}^2/\text{g}$ which is close to the value of $0.154 \text{ cm}^2/\text{g}$ previously found [26] and within the range of 0.21 to $0.13 \text{ cm}^2/\text{g}$ determined for 50 to 200 keV photons in PMMA, a compound of similar chemical composition [27].

3.3. Fluorescent images of the irradiated gel

The irradiated cell was scanned in 1 mm steps with the UV sheet orthogonal to the propagation (z) axis of the X-ray beam. The resulting 30 tomographic images of the fluorescence were used to construct a 3D translucent image of the beam within the gel as described in references [23] and [26]. This 3D representation can be viewed here in the form of a video either in full color or in blue-pixel gray-scale:

Video file links here: "Movie full color.MP4" or "Movie gray.MP4"

An end-on view of the fluorescent image is shown in Figure 3 where it is compared with the incident beam cross-section found using the radiochromic film. The same oval form of the beam cross section is apparent in the RFG gel. A pixel profile scan across the beam is shown in Figure 4. From this a penumbra value of 0.44 mm is found. This lies between the entrance and exit values of 0.41 mm and 0.54 mm found with the RC film. The spatial resolution of the profile for images taken in the x - y plane is 0.023 mm/pixel , which is considerably smaller than the penumbra value of 0.44 mm . As for the film measurements therefore, the penumbra is ascribed to edge-dispersion in the x-ray beam rather than spatial resolution of the measurements.

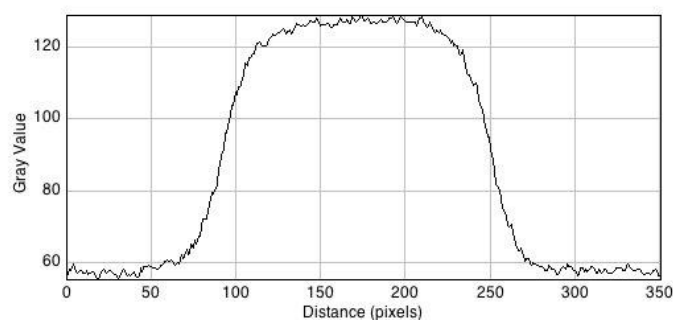


Figure 4. A pixel profile line scan across the center of the RFG gel image in Figure 3. The spatial resolution is 0.023 mm per pixel; the average 20-80% rise and fall value (the "penumbra") is 0.44 mm.

In Figure 5 (lower) a side view (y/z plane) of the fluorescence reconstruction is shown. This displays a gradual decrease in intensity with increasing depth in the gel as expected.

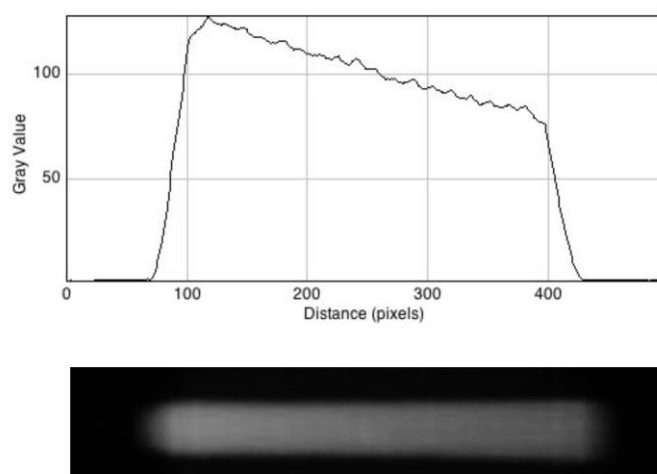


Figure 5. Lower: A still image of the reconstructed X-ray beam fluorescence side-on. Upper: An intensity profile of the image.

The decrease is quantified in the pixel profile scan in Figure 5 (Upper) which decreases by a factor of 0.63 over the length of the gel. This is close to the value of 0.67 that would be expected for the decrease in dose rate across the gel based on the value of $[Mp\delta]_{gel} = 0.296$ determined in section 3.2 and a conical expansion by 10%. Precise agreement might not be expected because of the *superlinear* dependence found for the fluorescence intensity on dose and the *sublinear* dependence found on dose rate [22]. These compensatory effects are the object of ongoing research into methods of making corrections to the experimental data required for dosimetry applications.

4. Conclusion

We have shown that it is possible to produce a 3-dimensional, fluorescent image of the energy deposited by a 3 mm beam of high-energy radiation in a gel medium of physical properties and dimensions close to those of the vitreous body of the human eye. A 3D video image of the beam, with submillimetre spatial resolution, can be produced in-house within minutes of irradiation using a portable tomographic fluorescence-scanning apparatus with refractive index matching. We intend to apply the method to the study of energy deposition by proton pencil beams and to the control of radiotherapy protocols and equipment when the Holland Proton Therapy Clinic is eventually commissioned (<http://www.hollandptc.nl/en/>).

References

1. Stannard, C.; Sauerwein, W.; Maree, G.; Lecuona, K. 2013 Radiotherapy for ocular tumours. *Eye (Lond)* **2013**, *27*(2), 119-127. doi: 10.1038/eye.2012.241.
2. Poder, J.; Corde, S. I-125 ROPES eye plaque dosimetry: Validation of a commercial 3D ophthalmic brachytherapy treatment planning system and independent dose calculation software with GafChromic EBT3 films. *Medical Physics* **2013**, *40*(12), 121709, 1-11. <http://ro.uow.edu.au/eispapers/1919>.
3. Eye Cancer: Treatment Options, <https://www.cancer.net/cancer-types/eye-cancer/treatment-options> [accessed 06 June 2018].
4. Radiation Therapy for Eye Cancer, <https://www.cancer.org/cancer/eye-cancer/treating/radiation-therapy.html> [accessed 06 June 2018].
5. The changing landscape of cancer therapy, <https://physicsworld.com/a/the-changing-landscape-of-cancer-therapy/> [accessed 06 June 2018].
6. McAuley, G.A.; Heczko, S.L.; Nguyen, T.; Slater, J.M.; Slater, J.D.; Wroe, A.J. Monte Carlo evaluation of magnetically focused proton beams for radiosurgery. *Phys. Med. Biol.* **2018**, *63*, 055010(13 pp). doi.org/10.1088/1361-6560/aaa92
7. Allen, A.M.; et al. An evidence based review of proton beam therapy: The report of ASTRO's emerging technology committee. *Radiotherapy and Oncology* **2012**, *103*, 8-11.
8. Goitein, G. Proton radiation therapy of ocular melanoma. *PTCOG 49 Teaching Course* **2010**.
http://www.ptcog.ch/archive/conference_p&t&v/PTCOG49/presentationsEW/18-4-3_Eye.pdf
9. Pasler, M.; Hernandez, V.; Jornet, N.; Clark, C.H. Novel methodologies for dosimetry audits: Adapting to advanced radiotherapy techniques. *Physics and Imaging in Radiation Oncology* **2018**, *5*, 76-84. doi.org/10.1016/j.phro.2018.03.002
10. Day, M.J.; Stein, G. Chemical effects of ionizing radiation in some gels. *Nature* **1950**, *166*, 146-7.
11. Baldock, C.; De Deene, Y.; Doran, S.; Ibbott, G.; Jirasek, A.; Lepage, M.; McAuley, K.B.; Oldham, M.; Schreiner, L.J. Polymer gel dosimetry. *Phys. Med. Biol.* **2010**, *55*, R1-63
12. Watanabe, Y.; Warmington, L.; Gopishankar, N. Three-dimensional radiation dosimetry using polymer gel and solid radiochromic polymer: From basics to clinical applications. *World J. Radiol.* **2017**, *9*(3), 112-125. doi: 10.4329/wjr.v9.i3.112
13. Vandecasteele, J.; De Deene, Y. Evaluation of radiochromic gel dosimetry and polymer gel dosimetry in a clinical dose verification. *Phys. Med. Biol.* **2013**, *58*, 6241-6252. doi: 10.1088/0031-9155/58/18/6241.
14. Schreiner, L.J. True 3D chemical dosimetry (gels, plastics): Development and clinical role. *J. Phys: Conf. Ser.* **2015**, *573*, 012003. doi:10.1088/1742-6596/573/1/012003.
15. Oldham, M. Radiochromic 3D Detectors. *J. Phys: Conf. Ser.* **2015**, *573*, 012006. doi:10.1088/1742-6596/573/1/012006.
16. Maryanski, M.J.; Schulz, R.J.; Ibbott, G.S.; Gatenby, J.C.; Xie, J.; Horton, D.; Gore, J.C. Magnetic resonance imaging of radiation dose distributions using a polymer gel dosimeter. *Phys. Med. Biol.* **1994**, *39*, 1437-1455.
17. Gore, J.C.; Ranade, M.; Maryanski, M.J.; Schulz, R.J. Radiation dose distributions in three dimensions from tomographic optical density scanning of polymer gels: I. Development of an optical scanner. *Phys. Med. Biol.* **1996**, *41*, 2695-2704.

18. Cameron, M.; Cornelius, I.; Cutajar, D.L.; Davis, J.A.; Rosenfeld, A.B.; Lerch, M.; Guatelli, S. Comparison of phantom materials for use in quality assurance of microbeam radiation therapy. *J. Synchrotron Radiation* **2017**, *24*(4), 866-876.
19. Kron, T.; Lehmann, J.; Greer P. Dosimetry of ionising radiation in modern radiation oncology. *Phys. Med. Biol.* **2016**, *61*, R167-R205. doi: 10.1088/0031-9155/61/14/R167.
20. Newton, J.; Oldham, M.; Thomas, A.; Li, Y.; Adamovics, J.; Kirsch, D.G.; Das, S. Commissioning a small-field biological irradiator using point, 2D, and 3D dosimetry techniques. *Med. Phys.* **2011**, *38*(12), 6754-6762. <https://doi.org/10.1118/1.3663675>.
21. Warman, J.M.; Luthjens, L.H.; de Haas, M.P. High-energy radiation monitoring based on radio-fluorogenic co-polymerization II: fixed fluorescent images of collimated x-ray beams using an RFCP gel. *Phys. Med. Biol.* **2011**, *56*, 1487-1508. doi: 10.1088/0031-9155/56/5/017.
22. Warman, J.M.; de Haas, M.P.; Luthjens, L.H.; Denkova, A.G.; Yao, T. A radio-fluorogenic polymer-gel makes fixed fluorescent images of complex radiation fields. *Polymers*, **2018**, *10*(6), 685. doi:10.3390/polym10060685.
23. Yao, T.; Gasparini, A.; de Haas, M.P.; Luthjens, L.H.; Denkova, A.G.; Warman, J.M. A tomographic UV-sheet scanning technique for producing 3D fluorescence images of x-ray beams in a radio-fluorogenic gel. *Biomed. Phys. Eng. Express* **2017**, *3*, 027004. <https://doi.org/10.1088/2057-1976/aa684b>
24. Warman, J.M.; de Haas, M.P.; Luthjens, L.H.; Denkova, A.G.; Kavatsyuk, O.; van Gothem, M-J.; Kiewiet, H.H.; Brandenburg, S. Fixed fluorescent images of an 80 MeV proton pencil beam. *Rad. Phys. Chem.* **2013**, *85*, 179-183. doi.org/10.1016/j.radphyschem.2012.11.011
25. Yao, T.; Luthjens, L.H.; Gasparini, A.; Warman, J.M. A study of four radiochromic films currently used for (2D) radiation dosimetry. *Rad. Phys. Chem.* **2017**, *133*, 37-44. <http://dx.doi.org/10.1016/j.radphyschem.2016.12.006>
26. Yao, T. 3D radiation dosimetry using a radio-fluorogenic gel. PhD thesis, 2017 Technische Universiteit Delft, ISBN 978-94-6295-563-9. doi:10.4233/uuid:e8590e7e-944c-4b4c-bc2b-3843400a9f85
27. Hubbell, J.H.; Seltzer, S.M. 1996 Tables of X-ray mass attenuation coefficients and mass energy-absorption coefficients from 1 keV to 20 MeV for elements $Z = 1$ to 92 and 48 additional substances of dosimetric interest. NISTIR #5632 (<http://www.nist.gov/pml/data/xraycoef/index.cfm>)