

Article

Phase Correction for Absorption Mode Two-dimensional Mass Spectrometry

Marc-André Delsuc^{1,2}, Kathrin Breuker³ and Maria A. van Agthoven^{3,*}

¹ INSERM U596, UMR 7104, Université de Strasbourg, 1 rue Laurent Fries, 67404 Illkirch-Graffenstaden, France; madelsuc@unistra.fr

² CASC4DE, Pôle API, 300 Bd. Sébastien Grant, 67400 Illkirch-Graffenstaden, France

³ Institute for Organic Chemistry, University of Innsbruck, Innrain 80/82, 6020 Innsbruck, Austria; kathrin.breuker@uibk.ac.at, maria.van-agthoven@uibk.ac.at

* Correspondence: maria.van-agthoven@uibk.ac.at

Abstract: Two-dimensional mass spectrometry (2D MS) is a method for tandem mass spectrometry that relies on manipulating ion motions to correlate precursor and fragment ion signals. 2D mass spectra are obtained by performing a Fourier transform in both the precursor ion mass-to-charge ratio (m/z) dimension and the fragment ion m/z dimension. The phase of the ion signals evolves linearly in the precursor m/z dimension and quadratically in the fragment m/z dimension. This study demonstrates that phase-corrected absorption mode 2D mass spectrometry improves signal-to-noise ratios by a factor of 2 and resolving power by a factor of 2 in each dimension compared to magnitude mode. Furthermore, phase correction leads to an easier differentiation between ion signals and artefacts, and therefore easier data interpretation.

Keywords: mass spectrometry; two-dimensional; tandem mass spectrometry; phase correction; absorption mode; data processing


1. Introduction

Two-dimensional mass spectrometry (2D MS) is a method for tandem mass spectrometry that relies on manipulating ion motions to correlate precursor and fragment ion signals [1-3]. Various methods for 2D MS have been developed for quadrupolar ion traps, linear ion traps, and Fourier transform ion cyclotron resonance mass spectrometry (FT-ICR MS) [4-9]. In 2D FT-ICR MS, the most frequently used pulse sequence is the one proposed by Pfändler *et al.* to modulate ion radii in the ICR cell before fragmentation [1-3,10,11]. The pulse sequence and data processing have been optimized for analytical use [12-15]. 2D FT-ICR MS has been used for applications ranging from small molecules and agrochemicals, to polymers, bottom-up and top-down proteomics [16-24]. 2D MS has also been adapted for high-resolution analysis of precursor ions over narrower mass-to-charge ratio (m/z) ranges [25].

One area in which the performance of 2D MS can be improved, since the method relies on Fourier transformation in both dimensions, is phase correction for absorption mode mass spectrometry. Until now, 2D mass spectra have been shown in magnitude mode. In one-dimensional FT-ICR MS, phase correction for absorption mode was proposed by Xian *et al.* and by Qi *et al.* [26,27]. Automation for phase correction in one-dimensional FT-ICR MS was achieved by Kilgour *et al.* [28-30]. Processing data sets in absorption mode has improved the performance of one-dimensional FT-ICR MS by a factor of 1.41 in signal-to-noise and a factor of 2 in resolving power, resulting in more complete and reliable analytical information for complex samples [31-37]. In 2D MS, we can therefore expect an improvement by a factor of $1.41 \times 1.41 = 2$ in signal-to-noise and in resolving power in each dimension.

A previous study has shown that the phase correction function is quadratic in the horizontal fragment ion dimension and linear in the vertical precursor ion dimension [38]. Here, we demonstrate how to perform phase correction on a narrowband 2D mass spectrum and we show how absorption mode 2D MS compares to magnitude mode.

2. Theory

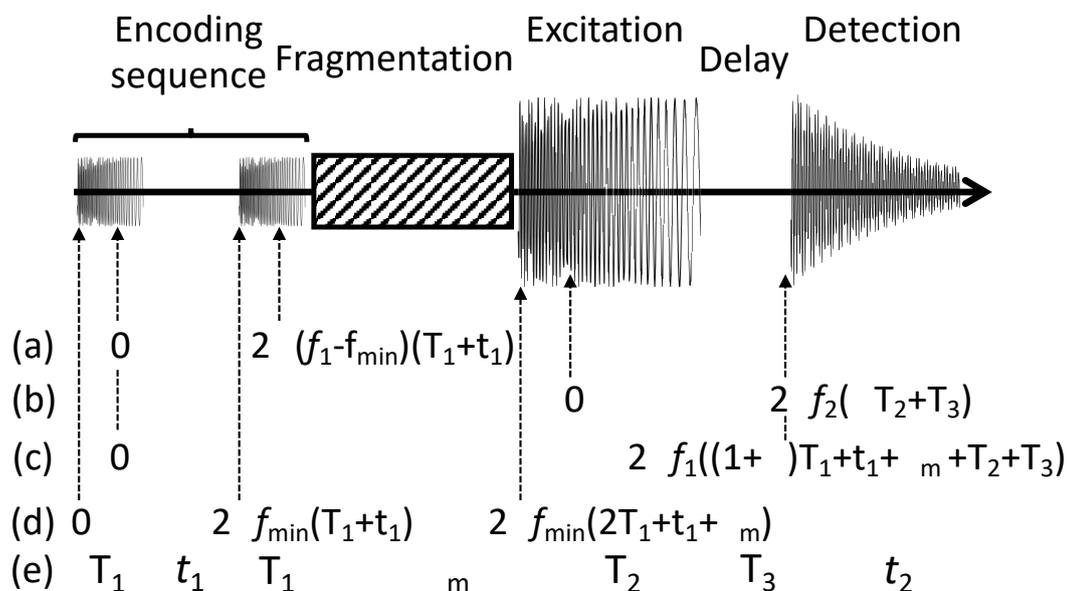

Scheme 1. Pulse sequence for two-dimensional mass spectrometry and evolution of phases for (a) precursor ion radii, (b) fragment ion motion, (c) unfragmented precursor ion motion, (d) excitation pulses. (e) Duration of each segment of the pulse sequence. The factor α (resp. β) is related to the moment that the swept frequency of the chirp reaches the cyclotron frequency of the fragment (resp. unfragmented precursor).

The pulse sequence for 2D MS is shown in Scheme 1. The chirp pulses used for the excitation are needed to excite a large range of frequencies for the fragment ions and they induce a quadratic phase dependence, requiring a quadratic phase correction in the fragment ion dimension [26,27,39]. In Scheme 1, the quadratic dependence of the phase of ion signals on their resonant cyclotron frequencies is expressed through the parameters α for fragment ions and β for precursor ions. In Bruker FT-ICR mass spectrometers, the initial phase of each pulse in the pulse sequence rotates with the minimum frequency of the pulses f_{\min} . Scheme 1 shows the initial phase of each pulse, which leads to a corresponding phase offset for the signals of ions that are excited from the center of the ICR cell in that pulse. As a rule, in Fourier transform mass spectrometry, a shift of origin induces a zero order phase, a delay induces a first order phase rotation, and a frequency-dependent excitation induces a second order phase rotation.

During the first pulse, the precursor ions are excited from the center of the ICR cell to higher radii and start accruing phase [38]. The initial phase of the first pulse is zero. The precursor ions rotate during the encoding delay t_1 at their own cyclotron frequency. The second pulse has a starting phase of $2\pi f_{\min}(T_1 + t_1)$. The phase difference between the second pulse and the precursor ion motion is $2\pi t_1(f_{\text{ICR}} - f_{\min})$ where f_{ICR} is the cyclotron frequency of the ion, f_{\min} is the minimum frequency in the pulse, and t_1 is the encoding delay. Therefore, according to the phase difference, precursors are excited to higher radii or de-excited towards the center of the ICR cell. The frequency of the precursor ion radius modulation is $f_{\text{ICR}} - f_{\min}$. At the end of the second pulse, the radius of the precursor ions can be expressed as [2,11,40]:

$$r(t_1) = r_0 \sqrt{2(1 + \cos 2\pi(f_{ICR} - f_{min})(t_1 - T_1))} \quad (\text{eq. 1})$$

After the second pulse, a fragmentation period τ_m with a method that has a maximum fragmentation efficiency at the center of the ICR cell, usually ECD or IRMPD, is applied to the precursor ions [14,22]. Ions at the center of the ICR cell are fragmented. The abundance of the fragment ions is modulated with the same frequency as the radius of the precursors, i.e. $f_{ICR} - f_{min}$. The third pulse has a starting phase of $2\pi f_{min}(2T_1 + t_1 + \tau_m)$ and excites all ions to high radius before detection. Fragment ions start accruing phase during the third pulse [38].

In the horizontal dimension, the phase $\varphi_{p,h}$ accrued by precursor ions that are not fully de-excited to the center of the ICR cell at the end of the second pulse can be expressed with a quadratic phase dependence as:

$$\varphi_{p,h}(f_1) = c_2' f_1^2 + c_1' f_1 + c_0' + 2\pi f_1 t_1 \quad (\text{eq. 2})$$

with $c_1' = c_1 + T_1 + \tau_m + T_2 + T_3$

in which c_0' , c_1 , and c_2' are the parameters for the quadratic phase incurred during excitation, f_1 is the cyclotron frequency of the ion, t_1 is the encoding delay, T_1 is the duration of the second pulse, τ_m is the fragmentation period, T_2 is the duration of the third pulse, and T_3 is the delay between excitation and detection [26,27,38].

The phase $\varphi_{f,h}$ accrued by fragment ions and unfragmented precursor ions that have been fully de-excited to the center of the ICR cell at the end of the second pulse can be expressed with a quadratic phase dependence as:

$$\varphi_{f,h}(f_2) = c_2'' f_2^2 + c_1'' f_2 + c_0'' \quad (\text{eq. 3})$$

with $c_0'' = c_0 + 2\pi f_{min}(2T_1 + t_1 + \tau_m)$

in which c_0 , c_1'' , and c_2'' are the parameters for the quadratic phase incurred during excitation, f_2 is the cyclotron frequency of the ion, t_1 is the encoding delay, T_1 is the duration of the first and the second pulse, τ_m is the fragmentation period.

In the vertical dimension, eq. 1 shows that the phase $\varphi_{p,v}$ for precursor ion signal can be expressed with a linear phase dependence as:

$$\varphi_{p,v}(f_1) = 2\pi(f_1 - f_{min})(t_1 - T_1) \quad (\text{eq. 4})$$

in which f_1 is the cyclotron frequency of the ion, t_1 is the encoding delay, f_{min} is the lowest frequency in the pulse, and T_1 is the duration of the second pulse.

Multiple studies have shown that in the vertical dimension, for fragmentation methods that have a maximum efficiency at the center of the ICR cell, the phase $\varphi_{f,v}$ of the fragment ion signal is shifted by π [38]. The phase of the fragment ion signal can therefore be expressed as:

$$\varphi_{f,v}(f_1) = 2\pi(f_1 - f_{min})(t_1 - T_1) + \pi \quad (\text{eq. 5})$$

in which f_1 is the cyclotron frequency of the precursor ion, t_1 is the encoding delay, f_{min} is the lowest frequency in the pulse, and T_1 is the duration of the second pulse.

Because signals have a t_1 amplitude modulation, a data set recorded in 2D mass spectrometry experiments requires processing using hypercomplex Fourier transformation [41-45]. The resulting spectrum is a 4-quadrant data set:

$$S(f_1, f_2) = RR(f_1, f_2) + iRI(f_1, f_2) + jIR(f_1, f_2) + kII(f_1, f_2) \quad (\text{eq. 6})$$

In which S is the signal in frequency domain, f_1 and f_2 are the frequencies, and i, j , and k are constants following the rules:

$$i^2 = j^2 = -1 \quad ; \quad k^2 = 1 \quad (\text{eq. 7})$$

$$i \cdot j = j \cdot i = k \quad (\text{eq. 8})$$

$$i \cdot k = k \cdot i = -j \quad (\text{eq. 9})$$

$$j \cdot k = k \cdot j = -i \text{ (eq. 10)}$$

With these rules, phase corrections can be applied independently to $S(f_1, f_2)$ along the f_1 and f_2 axes:

$$S(f_1, f_2)e^{i\varphi_1} = S(f_1, f_2)(\cos \varphi_1 + i \sin \varphi_1) \quad \text{(eq. 11)}$$

$$S(f_1, f_2)e^{j\varphi_2} = S(f_1, f_2)(\cos \varphi_2 + j \sin \varphi_2) \quad \text{(eq. 12)}$$

The phase corrections in the horizontal dimension and in the vertical dimensions can be applied independently from each other.

3. Experimental Methods

Sample Preparation

The sample used was an equimolar mixture of unmodified and modified (mono-, di-, and trimethylated) histone peptides that were C-terminal GK-biotinylated (AnaSpec, Fremont, CA, USA). Their sequence was ATKAARKSAP ATGGVKKPHR YRPGGK_{biotin} (human histone H3). The sample was prepared with the same protocol as described in a previous article.[25]

Instrument Parameters

Both the standard tandem mass spectrum and the two-dimensional mass spectrum were acquired on a 7 T Apex Ultra FT-ICR mass spectrometer (Bruker Daltonik, GmbH, Bremen, Germany) with an electrospray ion source operated in positive mode and direct injection at a flow rate of 70 μ L/hour. In both spectra, transients were acquired for 489.34 ms (512k datapoints) with an excitation pulse before detection with a frequency range of 535714.29 – 74728.13 Hz (corresponding to m/z 202.22 – 1450). The excitation pulse was made of 739 decrements of 624 Hz with 20 μ s per frequency. The amplitude of the excitation was 106 V_{pp} and the delay between excitation and detection was 3 ms.

For the standard tandem mass spectrum, ions were accumulated for 0.1 s in the first hexapole and 0.1 s in the second hexapole. In the quadrupole, ions were isolated at m/z 491 with an isolation window of m/z 30, and in the collision cell, they were activated with a 1.5 V collision energy before transfer to the Infinity ICR cell [46]. The fragmentation method was ECD, using a hollow cathode [47]. The heater was set at 1.3 A, the lens at 20 V, the bias at 1.7 V, and the irradiation lasted for 0.07 s.

The 2D mass spectrum was acquired in narrowband modulation mode [25]. The acquisition lasted 20 minutes. Accumulation was set at 0.2 s (first hexapole) and 0.2 s (second hexapole). Ions were quadrupole-isolated at m/z 491 with an isolation window of m/z 10. Ions were activated in the collision cell at 1.5 V collision energy. The ECD cathode parameters were 1.4 A (heater), 20 V (lens), 2.0 V (bias), and 0.06 s (irradiation). In the encoding sequence, the pulses had a frequency range of 535714.29 – 74728.13 Hz (corresponding to m/z 202.22 – 1450), with 739 decrements of 624 Hz with 1.0 μ s per frequency. The amplitude of the encoding pulses was 106 V_{pp}. The encoding delay incremented 1024 times by 50 μ s, corresponding to a 10 kHz bandwidth, with 1 scan per increment. The signal was folded over 14 times, leading to a frequency range of 214659.79 – 224659.79 Hz (corresponding to m/z 482.177 – 504.602 for precursor ion modulation) [25]. The parameters of the excitation-detection sequence were identical to the parameters used for the standard tandem mass spectrum, with transients lasting 489.34 ms (512k datapoints).

Data Processing

The standard one-dimensional tandem mass spectrum and the 2D mass spectrum were processed and visualized using the Spectrometry Processing Innovative Kernel software (SPIKE) developed by CASC4DE (Illkirch-Graffenstaden, France) and the University of Strasbourg. The programming language is 64-bit Python 3.7, used on an open-source platform distributed by the Python Software Foundation (Beaverton, OR, USA) [48]. The

processed 2D mass spectra were recorded in HDF5 file format. No denoising was applied to the dataset in magnitude or in absorption mode [12,13,15].

The transient for the one-dimensional tandem mass spectrum was apodised with a sine-bell window that was shifted, with a maximum of the bell at 15% of the transient, zero-filled twice, and Fourier transformed. The resulting spectrum was phase-corrected quadratically using a locally developed plugin to the SPIKE program (available at www.github.com/spike-project).

The program used for the data processing of the 2D mass spectrum in phase-corrected absorption mode is listed in the Appendix. Each transient in the 2D data set was apodised with a sine-bell window that was shifted, with a maximum of the bell at 15% of the transient, zero-filled twice and Fourier transformed. The modulation induced by the frequency generator was then removed by a complex rotation of the opposite frequency in the vertical dimension along the t_1 delay. The demodulation frequency was determined to be 74659.79 Hz. The exact demodulation frequency was offset by 68 Hz from the lowest frequency entered in the Apex Control software. The correct demodulation frequency was measured by processing the 2D mass spectrum with the nominal frequency entered in the software, which causes peak-splitting on the autocorrelation line, and measuring the frequency difference between the split peaks. Digital demodulation with the corrected frequency eliminated the peak-splitting [17]. The parameters determined for the one-dimensional tandem mass spectrum for quadratic phase correction were then applied to each row in the spectrum. The imaginary part of each row of the data set was then removed to reduce the computer memory burden. Then, each column of the data set was apodised with a slightly shifted sine-bell window (with a maximum of the bell at 15% of the transient), zero-filled twice and Fourier transformed. The theoretical linear phase correction determined above was applied on each column without modification. The imaginary part of the signal in each column was dropped and the dataset stored on disk.

The same 2D MS data set was processed in magnitude mode with identical apodisation and digital demodulation. However, due to the limitations of computer memory, the data-set was only zero-filled once in each dimension.

4. Results and Discussion

Figure 1 shows the result of quadratic phase correction with the SPIKE plugin for the one-dimensional ECD tandem mass spectrum of the four histone peptides. Although phase correction for FT-ICR mass spectra has been fully automated, this program requires user optimization [28,29,32,33,49]. The phase correction method is based on initial phase correction of small regions of the spectrum with linear phase functions, in a similar way to the methods proposed by Xian *et al.* [26] and Qi *et al.* [27]. The coefficients of the overall quadratic phase correction function are estimated using the slope and offsets of these local linear phase correction functions, by using the fact that these linear phase functions are tangents of the overall quadratic phase function. The user can then optimize the coefficients until the whole spectrum is properly phase-corrected.

Figure 1a shows the absorption mode mass spectrum before phase correction and Fig. 1b shows the absorption mode mass spectrum after phase correction. Fig. 1b shows that the signal for all the ions in the mass spectrum has been properly corrected. An insert shows a zoom-in on the isotopic distribution of the z_{24}^{4+} fragment of the monomethylated histone peptide and compares the phase-corrected absorption mode mass spectrum to the magnitude mode mass spectrum. Both the resolving power and the signal-to-noise ratio

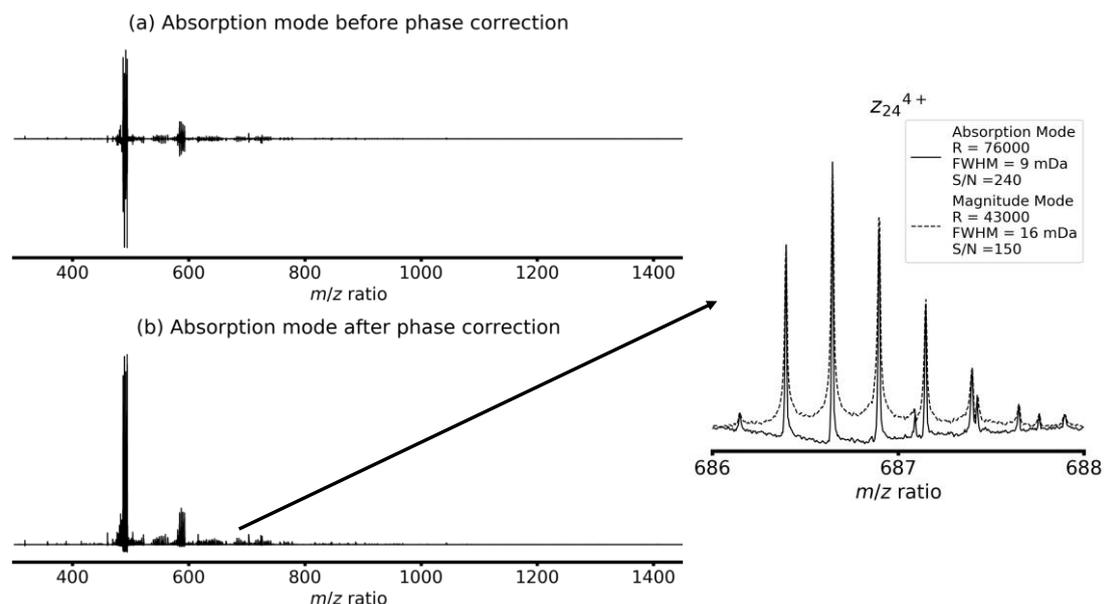


Figure 1. Tandem mass spectrum of the $[M+6H]^{6+}$ histone peptides with ECD fragmentation in absorption mode (a) before phase correction and (b) after phase correction. Insert: zoom-in on the z_{24}^{4+} fragment ion isotopic distribution of the monomethylated histone peptide (K7 1m), comparison between magnitude mode and phase-corrected absorption mode (FWHM: full-width at half-maximum).

are almost double for the phase corrected absorption mode spectrum than for the magnitude mode spectrum, as predicted by theory [26,27].

The one-dimensional tandem mass spectrum was acquired with excitation pulse parameters and an excite-detect delay that was identical to the excitation pulse and the excite-detect delay of the 2D MS pulse sequence. Qi *et al.* have showed that the phase correction function is very stable with experimental conditions [50]. The phase correction function determined for the one-dimensional tandem mass spectrum can therefore also be used for the phase correction of the fragment ion signals in the 2D mass spectrum, which are, analytically, the most informative signals [38].

The only difference between the excitation pulse for the tandem mass spectrum and the 2D mass spectrum is the initial phase of the pulse, which is determined by the continuous phase pulse generator. As is shown in Scheme 1, the phase shift of the excitation pulse in the 2D MS experiment is $2\pi f_{\min}(2T_1+t_1+\tau_m)$, in which f_{\min} is the minimum frequency in the pulse, T_1 is the duration of the first pulse, τ_m the irradiation period, and t_1 is the incremental delay. $2\pi f_{\min}(2T_1+\tau_m)$ is constant throughout the experiment (and can be corrected with a constant phase offset in the phase correction function), but $2\pi f_{\min}t_1$ is different for each transient.

Digital demodulation eliminates the phase contribution of $2\pi f_{\min}t_1$ in each transient. In magnitude mode, digital demodulation is used to reduce the number of harmonics visible in the 2D mass spectrum [11,17]. Here, by applying digital demodulation before the quadratic phase correction in the horizontal dimension, we can eliminate the effect of the continuous phase pulse generator on the phase of fragment ion signals.

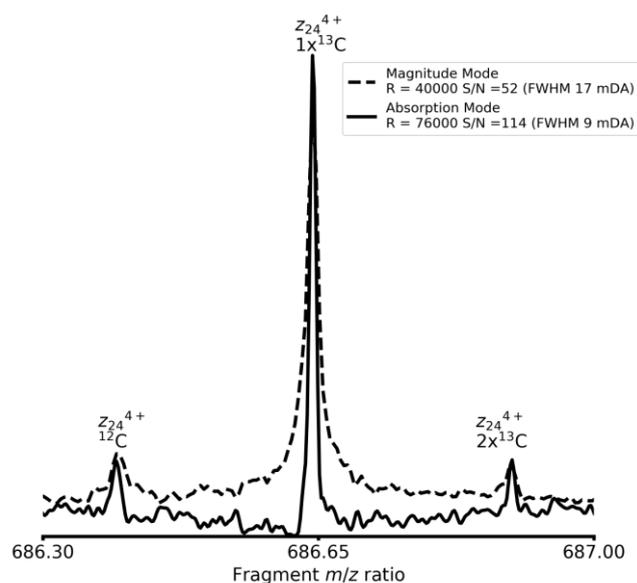


Figure 2. Extracted fragment ion scan from the 2D mass spectrum for the $1\times^{13}\text{C}$ isotope of $(\text{M}+6\text{H})^{6+}$ ions of the monomethylated histone peptide (K7 1m) at m/z 489.453, zoom-in on fragment ion z_{24}^{4+} , comparison between absorption mode and magnitude mode.

Figure 2 focuses on the extracted fragment ion scan of the $1\times^{13}\text{C}$ isotope of $(\text{M}+6\text{H})^{6+}$ ions of the monomethylated histone peptide (K7 1m). The fragment z_{24}^{4+} contains 24 out of the 26 residues of the peptide. Consequently, if the precursor ion contains exactly one ^{13}C , then the probability of z_{24}^{4+} retaining the ^{13}C is very high [11,25,51-53]. In Figure 2, the relative intensity of the $1\times^{13}\text{C}$ isotope of z_{24}^{4+} is much higher than the relative intensity of the ^{12}C isotope. We can also see a peak for the $2\times^{13}\text{C}$ isotope of z_{24}^{4+} , which is caused by scintillation noise from the fragment of the $2\times^{13}\text{C}$ isotope of the precursor ion. The isotopic distribution shown in Figure 2 is a consequence of the precursor ion signals being isotopically resolved in the vertical dimension. In the horizontal dimension, the phase-corrected absorption mode has doubled the resolving power and signal-to-noise ratio of the magnitude mode, as expected [26,27].

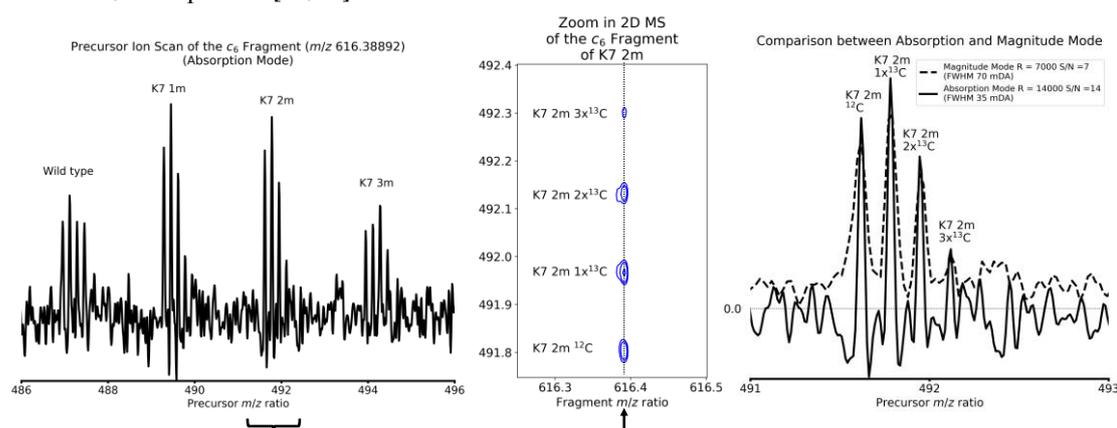


Figure 3. Precursor ion scan extracted from the absorption mode 2D mass spectrum for the ^{12}C isotope of the c_6 fragment of the histone peptides (m/z 616.38892), zoom-in on the c_6 fragment ion isotopic distribution in the 2D mass spectrum for the dimethylated histone peptide (K7 2m), comparison between the absorption mode and magnitude mode of the precursor ion scan of the c_6 fragment.

Figure 3 shows the extracted precursor ion scan of the ^{12}C isotope of the c_6 fragment of the histone peptides. Since the modifications are all on the 7th residue from the N-terminus, all histone peptides in the sample have identical c_6 fragments. This precursor ion scan is therefore an appropriate column of the data set to test the linear phase correction function. Equations 4 and 5 predict that the phase correction function has a slope of $f_N T_1$, in which f_N represents the vertical Nyquist frequency (i.e. 10 kHz in the present experiment) and T_1 is the duration of the first pulse (i.e. 739 μs). Therefore, the theoretical first order phase correction should be of 7.39 turns over the whole spectrum. The resulting spectrum is well-phased, but we observed that 7.8 turns give slightly better results (see Appendix). Figure 3 (left) shows that the phase correction function yields a well-corrected spectrum in the vertical dimension. A comparison with the extracted precursor ion scan from the magnitude mode spectrum (Fig. 3 right) shows that the absorption mode spectrum has doubled the resolving power and signal-to-noise ratio compared to the magnitude mode spectrum, as is predicted [26,27]. However, as this experiment was acquired in narrowband mode vertically, the frequency bandwidth is about twenty times narrower than in broadband 2D mass spectra, which may lead to a different phase correction [25].

The zoom-in on the isotopic distribution of the c_6 fragment of the dimethylated histone peptide (Fig. 3 centre) shows that the peaks are very well resolved. The full-width at half-maximum (FWHM) of the peaks is approximately 35 mDa ($R = 14000$ at m/z 490), which is sufficient to isotopically resolve the fragments of biomolecules up to 14 kDa.

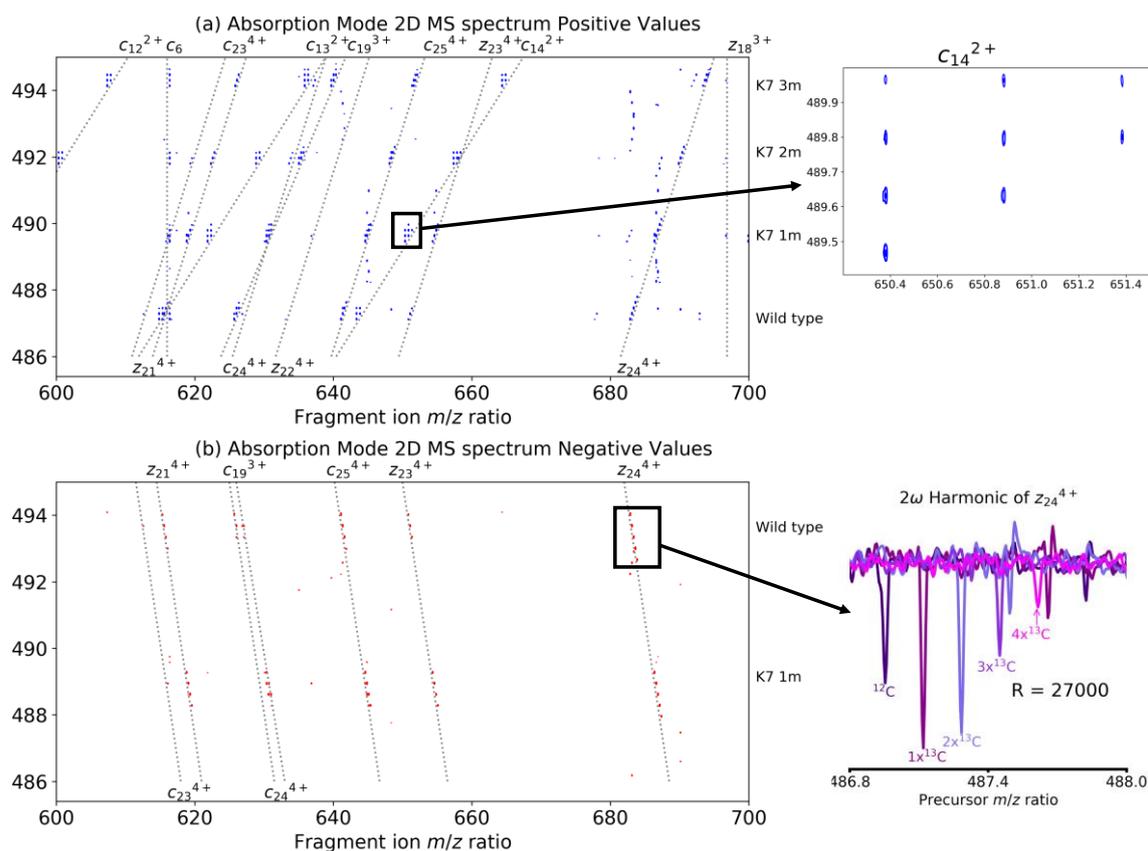


Figure 4. Phase-corrected absorption mode 2D mass spectrum of histone peptides, zoomed in between m/z 600-700 horizontally and m/z 485-495 vertically, (a) positive values plotted (insert: zoom-in on the isotopic distribution of the c_{14}^{2+} fragment of the methylated histone peptide) and (b) negative values plotted (insert: vertical precursor ion scans of the isotopic distribution of z_{24}^{4+} of the unmodified histone peptide, with frequency-to-mass conversion for the 2ω harmonic).

Figure 4a shows a zoom-in on the 2D mass spectrum in phase-corrected absorption mode with only the positive values in the 2D mass spectrum. A similar 2D mass spectrum

of the same sample was analyzed in detail in a previous article [25]. We notice that all isotopic distributions are isotopically resolved in both dimensions. An insert with a zoom-in on the isotopic distribution of the c_{14}^{2+} fragment of the monomethylated histone peptide shows that clearly.

Figure 4a shows mostly fragment ion peaks with very few artefacts. Figure 4b shows the negative values in the same region, which correspond to the 2ω harmonic of the ion signal in the vertical dimension [14]. The modulation frequency of the unmodified and the monomethylated peptides is between 146.34 and 147.34 kHz. Since the frequency range is 10 kHz, this leads to 14 foldovers for these signals. Because of the amplitude modulation of the signal in 2D MS and the real Fourier transform used during processing along the vertical axis, every time a signal is folded over in the 2D mass spectrum, the phase is shifted by 180° (or π radians). In this experiment, the signal has been folded over 14 times, and the phase is shifted by a multiple of 360° . The frequencies for the 2ω harmonic are between 292.68 and 294.68 kHz, so the signal has been folded over 29 times. Because the signal has been folded over an odd number of times, the 2ω harmonic of each dissociation line is a decreasing hyperbola, but over an m/z 3 range, it may appear linear [11]. The phase of the 2ω harmonic has been shifted by 29 times 180° , and the peaks corresponding to the 2ω harmonic have negative intensities, which simplifies data visualization and interpretation of the 2D mass spectrum.

The insert in Figure 4b shows the 2ω harmonic peaks for the isotopes for the z_{24}^{4+} fragment of the unmodified histone peptide with frequency-to-mass conversion that has been adapted to the 2ω harmonics. An additional phase correction of -33° was applied to the extracted precursor ion scans to correctly phase the 2ω harmonic peaks. As has been discussed in a previous article, the harmonic signals in a 2D mass spectrum can be used to increase the resolving power, just like they can in one-dimensional mass spectra [25,54-57]. Here, we almost double the resolving power from $R = 14,000$ to $R = 27,000$.

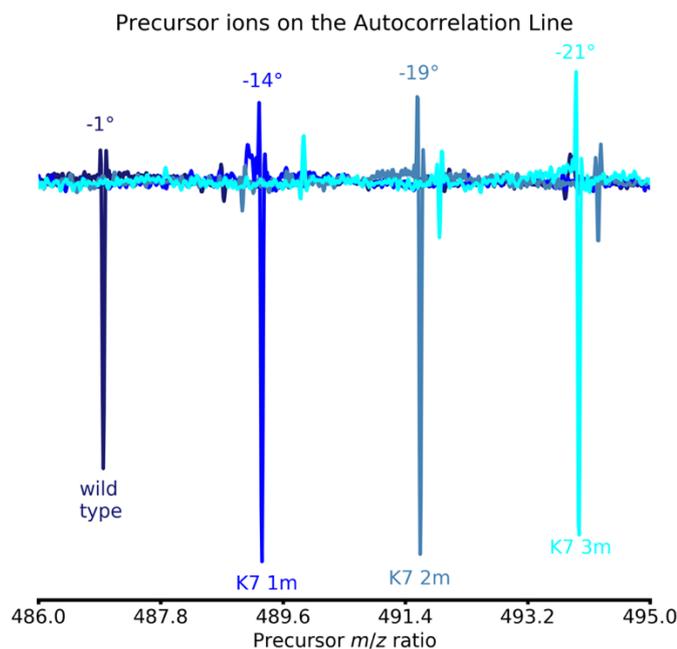


Figure 5. Extracted precursor ion scans for the ^{12}C isotopes of the four histone peptides from the phase-corrected absorption mode 2D mass spectrum.

Figure 5 shows the precursor ion scans for the ^{12}C isotopes of all four histone peptides on the autocorrelation line of the 2D mass spectrum. A comparison between equations 2 and 4 shows that, in the horizontal fragment ion dimension, the phase of precursor ion signals behaves differently from the phase of fragment ion signals, and that the phase

correction function for precursor ion signals depends on t_1 . Furthermore, as shown in equations 2 and 3, in the vertical precursor ion dimension, the phase of precursor ion signals is shifted by -180° compared to the phase of fragment ion signals [38]. Figure 5 confirms that, with phase correction functions that aim to correct the phases of fragment ion signals, precursor ion peaks on the autocorrelation line have negative intensities, and that their phase shifts with their cyclotron frequency (and their m/z ratio).

5. Conclusions

In this study, we have for the first time obtained a phase-corrected absorption mode two-dimensional mass spectrum by performing a quadratic phase correction in the horizontal fragment ion dimension and a linear phase correction in the precursor ion dimension. The resulting 2D mass spectrum shows the expected performance improvements in terms of resolving power and signal-to-noise ratio [26,27,38]. An added benefit of phase correction is the clear differentiation between “ground state” ion signals and folded-over harmonics, which, in our case, have negative intensities. This result can be expanded to broadband 2D MS, for harmonics that have been folded over. Careful experimental design can lead to good use of this effect.

Phase-corrected absorption mode narrowband 2D MS is shown here to enable isotopically resolved tandem mass spectrometry for biomolecules up to 14 kDa on a 7 T FT-ICR mass spectrometer. This performance opens the way for the identification, location, and relative quantification, of modifications such as citrullination or de-amidation in peptides and proteins by two-dimensional mass spectrometry [25,58,59]. In future studies, phase correction for 2D MS needs to be expanded to broadband 2D mass spectra and automated for easy data processing.

Author Contributions: All authors have contributed to the manuscript equally, read and agreed to the published version of the manuscript.

Funding: This research was funded by Der Wissenschaftsfonds (Austrian Science Fund, FWF) with the Lise Meitner Fellowship project M 2757-B.

Data Availability Statement: In this section, please provide details regarding where data supporting reported results can be found, including links to publicly archived datasets analyzed or generated during the study. Please refer to suggested Data Availability Statements in section “MDPI Research Data Policies” at <https://www.mdpi.com/ethics>. You might choose to exclude this statement if the study did not report any data.

Acknowledgments: The authors thank Ms. Sarah Heel, Mr. Michael Palasser, and Dr. Christopher A. Wootton for helpful conversations. M.A.v.A. and K.B. thank Der Wissenschaftsfonds (Austrian Science Fund, FWF) for the Lise Meitner Fellowship project M 2757-B.

Conflicts of Interest: The authors declare no conflict of interest.

Appendix A

Data processing for phase correction absorption mode 2D mass spectrum

```
# Import necessary modules
import spike
from spike.File import Apex
# Load 2D data set:
d = Apex.Import_2D("histonepeptide_2D_000002.d")
# Apodisation with a sine bell with a maximum at 15% of the transient, double zero-filling in #the
horizontal dimension, Fourier transform in the horizontal dimension
d.apod_sin(axis=2,maxi=0.15).chsize(d.size1,4*d.size2).rfft(axis=
2)
# Digital demodulation by multiplying every row by  $e^{-2\pi j f_{min} t_1}$ :
d.flipphase(0.0, 180*d.axis1.htoi(74659.79), axis = 1)
# Quadratic phase correction in the horizontal dimension with  $-9/360+564(f_2/f_N)+4595.7(f_2/f_N)^2$ *
```

```

d.phase(-9, 564.0, 4595.7, 0.0, axis = 2)
# Discard of the imaginary part of the data in the horizontal dimension
d.real(axis=2)
# Apodisation with a sine bell with a maximum at 15% of the transient, double zero-filling in the
vertical dimension, Fourier transform in the vertical dimension
d.apod_sin(axis=1,maxi=0.15).chsize(4*d.size1,d.size2).rfft(axis=
1)
# Linear phase correction in the vertical dimension with 59.9/360+7.8(fi/fN):*
d.phase(59.9, 7.8, 0.0, 0.00, axis=1)
# Discard of the imaginary part of the data in the vertical dimension
d.real(axis=1)
# Offset of the frequencies for narrowband 2D mass spectrometry
offset = 74659.79
d.axis1.offsetfreq = 14*d.axis1.specwidth + offset
d.axis1.leftpoint = 0

```

* In the phase function the first variable is the zero order correction, in degrees. The second and third variable are resp. the first and second order corrections, and they are expressed in number of turns throughout the spectrum.

References

- Pfändler, P.; Bodenhausen, G.; Rapin, J.; Houriet, R.; Gäumann, T. Two-dimensional Fourier transform ion cyclotron resonance mass spectrometry. *Chem. Phys. Lett.* **1987**, *138*(2-3), 195-200. doi:10.1016/0009-2614(87)80367-6
- Pfändler, P.; Bodenhausen, G.; Rapin, J.; Walser, M. E.; Gäumann, T. Broad-band two-dimensional Fourier transform ion cyclotron resonance. *J. Am. Chem. Soc.* **1988**, *110*(17), 5625-5628. doi:10.1021/ja00225a006
- Bensimon, M.; Zhao, G.; Gäumann, T. A method to generate phase continuity in two-dimensional Fourier transform ion cyclotron resonance mass spectrometry. *Chem. Phys. Lett.* **1989**, *157*(1-2), 97-100. doi:10.1016/0009-2614(89)87215-X
- Snyder, D. T.; Szalwinski, L. J.; Wells, J. M.; Cooks, R. G. Logical MS/MS scans: a new set of operations for tandem mass spectrometry. *Analyst* **2018**, *143*(22), 5438-5452. doi:10.1039/C8AN01661E
- Snyder, D. T.; Szalwinski, L. J.; St. John, Z.; Cooks, R. G. Two-Dimensional Tandem Mass Spectrometry in a Single Scan on a Linear Quadrupole Ion Trap. *Anal. Chem.* **2019**, *91*(21), 13752-13762. doi:10.1021/acs.analchem.9b03123
- Szalwinski, L. J.; Holden, D. T.; Morato, N. M.; Cooks, R. G. 2D MS/MS Spectra Recorded in the Time Domain Using Repetitive Frequency Sweeps in Linear Quadrupole Ion Traps. *Anal. Chem.* **2020**, *92*(14), 10016-10023. doi:10.1021/acs.analchem.0c01719
- Driver, T.; Cooper, B.; Ayers, R.; Pipkorn, R.; Patchkovskii, S.; Averbukh, V.; Klug, D. R.; Marangos, J. P.; Frasiniski, L. J.; Edelson-Averbukh, M. Two-Dimensional Partial-Covariance Mass Spectrometry of Large Molecules Based on Fragment Correlations. *Phys. Rev. X* **2020**, *10*(4), 041004. doi:10.1103/PhysRevX.10.041004
- Szalwinski, L. J.; Cooks, R. G. Complex mixture analysis by two-dimensional mass spectrometry using a miniature ion trap. *Talanta Open* **2021**, *3*, 100028. doi:10.1016/j.talo.2020.100028
- van Agthoven, M. A.; O'Connor, P. B. Two-dimensional mass spectrometry in a linear ion trap, an in silico model. *Rapid Comm. Mass Spectrom.* **2017**, *31*(8), 674-684. doi:10.1002/rcm.7836
- van Agthoven, M. A.; Delsuc, M.-A.; Bodenhausen, G.; Rolando, C. Towards analytically useful two-dimensional Fourier transform ion cyclotron resonance mass spectrometry. *Anal. Bioanal. Chem.* **2013**, *405*(1), 51-61. doi:10.1007/s00216-012-6422-8
- van Agthoven, M. A.; Lam, Y. P. Y.; O'Connor, P. B.; Rolando, C.; Delsuc, M.-A. Two-dimensional mass spectrometry: new perspectives for tandem mass spectrometry. *Eur. Biophys. J.* **2019**, *48*(3), 213-229. doi:10.1007/s00249-019-01348-5
- van Agthoven, M. A.; Coutouly, M.-A.; Rolando, C.; Delsuc, M.-A. Two-dimensional Fourier transform ion cyclotron resonance mass spectrometry: reduction of scintillation noise using Cadzow data processing. *Rapid. Commun. Mass Spectrom.* **2011**, *25*(11), 1609-1616. doi:10.1002/rcm.5002
- Chiron, L.; van Agthoven, M. A.; Kieffer, B.; Rolando, C.; Delsuc, M.-A. Efficient denoising algorithms for large experimental datasets and their applications in Fourier transform ion cyclotron resonance mass spectrometry. *Proc. Natl. Acad. Sci. U. S. A.* **2014**, *111*(4), 1385-1390. doi:10.1073/pnas.1306700111
- van Agthoven, M. A.; Chiron, L.; Coutouly, M.-A.; Sehgal, A. A.; Pelupessy, P.; Delsuc, M.-A.; Rolando, C. Optimization of the discrete pulse sequence for two-dimensional FT-ICR mass spectrometry using infrared multiphoton dissociation. *Int. J. Mass Spectrom.* **2014**, *370*(0), 114-124. doi:10.1016/j.ijms.2014.06.019
- Bray, F.; Bouclon, J.; Chiron, L.; Witt, M.; Delsuc, M.-A.; Rolando, C. Nonuniform Sampling Acquisition of Two-Dimensional Fourier Transform Ion Cyclotron Resonance Mass Spectrometry for Increased Mass Resolution of Tandem Mass Spectrometry Precursor Ions. *Anal. Chem.* **2017**, *89*(17), 8589-8593. doi:10.1021/acs.analchem.7b01850
- van Agthoven, M. A.; Delsuc, M.-A.; Rolando, C. Two-dimensional FT-ICR/MS with IRMPD as fragmentation mode. *Int. J. Mass Spectrom.* **2011**, *306*(2-3), 196-203. doi:10.1016/j.ijms.2010.10.034

17. van Agthoven, M. A.; Chiron, L.; Coutouly, M.-A.; Delsuc, M.-A.; Rolando, C. Two-Dimensional ECD FT-ICR Mass Spectrometry of Peptides and Glycopeptides. *Anal. Chem.* **2012**, *84*(13), 5589-5595. doi:10.1021/ac3004874
18. van Agthoven, M. A.; Barrow, M. P.; Chiron, L.; Coutouly, M.-A.; Kilgour, D.; Wootton, C. A.; Wei, J.; Soulby, A.; Delsuc, M.-A.; Rolando, C.; O'Connor, P. B. Differentiating Fragmentation Pathways of Cholesterol by Two-Dimensional Fourier Transform Ion Cyclotron Resonance Mass Spectrometry. *J. Am. Soc. Mass Spectrom.* **2015**, *26*(12), 2105-2114. doi:10.1007/s13361-015-1226-7
19. Floris, F.; van Agthoven, M.; Chiron, L.; Soulby, A. J.; Wootton, C. A.; Lam, Y. P. Y.; Barrow, M. P.; Delsuc, M.-A.; O'Connor, P. B. 2D FT-ICR MS of Calmodulin: A Top-Down and Bottom-Up Approach. *J. Am. Soc. Mass Spectrom.* **2016**, *27*(9), 1531-1538. doi:10.1007/s13361-016-1431-z
20. van Agthoven, M. A.; Wootton, C. A.; Chiron, L.; Coutouly, M.-A.; Soulby, A.; Wei, J.; Barrow, M. P.; Delsuc, M.-A.; Rolando, C.; O'Connor, P. B. Two-Dimensional Mass Spectrometry for Proteomics, a Comparative Study with Cytochrome c. *Anal. Chem.* **2016**, *88*(8), 4409-4417. doi:10.1021/acs.analchem.5b04878
21. Floris, F.; van Agthoven, M. A.; Chiron, L.; Wootton, C. A.; Lam, P. Y. Y.; Barrow, M. P.; Delsuc, M.-A.; O'Connor, P. B. Bottom-Up Two-Dimensional Electron-Capture Dissociation Mass Spectrometry of Calmodulin. *J. Am. Soc. Mass Spectrom.* **2018**, 207-210. doi:10.1007/s13361-017-1812-y
22. van Agthoven, M. A.; Lynch, A. M.; Morgan, T. E.; Wootton, C. A.; Lam, Y. P. Y.; Chiron, L.; Barrow, M. P.; Delsuc, M.-A.; O'Connor, P. B. Can Two-Dimensional IR-ECD Mass Spectrometry Improve Peptide de Novo Sequencing? *Anal. Chem.* **2018**, *90*(5), 3496-3504. doi:10.1021/acs.analchem.7b05324
23. Paris, J.; Morgan, T. E.; Wootton, C. A.; Barrow, M. P.; O'Hara, J.; O'Connor, P. B. Facile Determination of Phosphorylation Sites in Peptides Using Two-Dimensional Mass Spectrometry. *Anal. Chem.* **2020**. doi:10.1021/acs.analchem.0c00884
24. Marzullo, B. P.; Morgan, T. E.; Wootton, C. A.; Perry, S. J.; Saeed, M.; Barrow, M. P.; O'Connor, P. B. Advantages of Two-Dimensional Electron-Induced Dissociation and Infrared Multiphoton Dissociation Mass Spectrometry for the Analysis of Agrochemicals. *Anal. Chem.* **2020**, *92*(17), 11687-11695. doi:10.1021/acs.analchem.0c01585
25. Halper, M.; Delsuc, M.-A.; Breuker, K.; van Agthoven, M. A. Narrowband Modulation Two-Dimensional Mass Spectrometry and Label-Free Relative Quantification of Histone Peptides. *Anal. Chem.* **2020**, *92*(20), 13945-13952. doi:10.1021/acs.analchem.0c02843
26. Xian, F.; Hendrickson, C. L.; Blakney, G. T.; Beu, S. C.; Marshall, A. G. Automated Broadband Phase Correction of Fourier Transform Ion Cyclotron Resonance Mass Spectra. *Anal. Chem.* **2010**, *82*(21), 8807-8812. doi:10.1021/ac101091w
27. Qi, Y.; Thompson, C. J.; Van Orden, S. L.; O'Connor, P. B. Phase correction of Fourier transform ion cyclotron resonance mass spectra using MatLab. *J. Am. Soc. Mass Spectrom.* **2011**, *22*(1), 138-147. doi:10.1007/s13361-010-0006-7
28. Kilgour, D. P. A.; Wills, R.; Qi, Y.; O'Connor, P. B. Autophaser: An Algorithm for Automated Generation of Absorption Mode Spectra for FT-ICR MS. *Anal. Chem.* **2013**, *85*(8), 3903-3911. doi:10.1021/ac303289c
29. Kilgour, D. P. A.; Nagornov, K. O.; Kozhinov, A. N.; Zhurov, K. O.; Tsybin, Y. O. Producing absorption mode Fourier transform ion cyclotron resonance mass spectra with non-quadratic phase correction functions. *Rapid Commun. Mass Spectrom.* **2015**, *29*(11), 1087-1093. doi:10.1002/rcm.7200
30. Kilgour, D. P. A.; Van Orden, S. L.; Tran, B. Q.; Goo, Y. A.; Goodlett, D. R. Producing Isotopic Distribution Models for Fully Apodized Absorption Mode FT-MS. *Anal. Chem.* **2015**, *87*(11), 5797-5801. doi:10.1021/acs.analchem.5b01032
31. Qi, Y.; Li, H.; Wills, R. H.; Perez-Hurtado, P.; Yu, X.; Kilgour, D. P. A.; Barrow, M. P.; Lin, C.; O'Connor, P. B. Absorption-Mode Fourier Transform Mass Spectrometry: The Effects of Apodization and Phasing on Modified Protein Spectra. *J. Am. Soc. Mass Spectrom.* **2013**, *24*(6), 828-834. doi:10.1007/s13361-013-0600-6
32. Smith, D. F.; Kilgour, D. P. A.; Konijnenburg, M.; O'Connor, P. B.; Heeren, R. M. A. Absorption mode FTICR mass spectrometry imaging. *Anal. Chem.* **2013**, *85*(23), 11180-11184. doi:10.1021/ac403039t
33. Kilgour, D. P. A.; Neal, M. J.; Soulby, A. J.; O'Connor, P. B. Improved optimization of the Fourier transform ion cyclotron resonance mass spectrometry phase correction function using a genetic algorithm. *Rapid Commun. Mass Spectrom.* **2013**, *27*(17), 1977-1982. doi:10.1002/rcm.6658
34. Qi, Y.; Witt, M.; Jertz, R.; Baykut, G.; Barrow, M. P.; Nikolaev, E. N.; O'Connor, P. B. Absorption-mode spectra on the dynamically harmonized Fourier transform ion cyclotron resonance cell. *Rapid Commun. Mass Spectrom.* **2012**, *26*(17), 2021-2026. doi:10.1002/rcm.6311
35. Qi, Y.; Barrow, M. P.; Li, H.; Meier, J. E.; Van Orden, S. L.; Thompson, C. J.; O'Connor, P. B. Absorption-Mode: The Next Generation of Fourier Transform Mass Spectra. *Anal. Chem.* **2012**, *84*(6), 2923-2929. doi:10.1021/ac3000122
36. Cho, Y.; Qi, Y.; O'Connor, P. B.; Barrow, M. P.; Kim, S. Application of Phase Correction to Improve the Interpretation of Crude Oil Spectra Obtained Using 7 T Fourier Transform Ion Cyclotron Resonance Mass Spectrometry. *J. Am. Soc. Mass Spectrom.* **2014**, *25*(1), 154-157. doi:10.1007/s13361-013-0747-1
37. Qi, Y.; Luo, R.; Schrader, W.; Volmer, D. A. Application of phase correction to improve the characterization of photooxidation products of lignin using 7 Tesla Fourier-transform ion cyclotron resonance mass spectrometry. *FACETS* **2017**, *2*(1), 461-475. doi:10.1139/facets-2016-0069
38. van Agthoven, M. A.; Kilgour, D. P. A.; Lynch, A. M.; Barrow, M. P.; Morgan, T. E.; Wootton, C. A.; Chiron, L.; Delsuc, M.-A.; O'Connor, P. B. Phase relationships in two-dimensional mass spectrometry. *J. Am. Soc. Mass Spectrom.* **2019**, *30*(12), 2594-2607. doi:10.1021/jasms.8b06276
39. Comisarow, M. B.; Marshall, A. G. Frequency-sweep Fourier transform ion cyclotron resonance spectroscopy. *Chem. Phys. Lett.* **1974**, *26*(4), 489-490. doi:10.1016/0009-2614(74)80397-0

40. Guan, S.; Jones, P. R. A theory for two-dimensional Fourier-transform ion cyclotron resonance mass spectrometry. *J. Chem. Phys.* **1989**, *91*(9), 5291-5295. doi:10.1063/1.457575
41. Delsuc, M.-A. Spectral Representation of 2D NMR Spectra by Hypercomplex Numbers. *J. Mag. Res.* **1988**, *77*, 119-124. doi:10.1016/0022-2364(88)90036-4
42. Schuyler, A. D.; Maciejewski, M. W.; Stern, A. S.; Hoch, J. C. Formalism for hypercomplex multidimensional NMR employing partial-component subsampling. *J. Mag. Res.* **2013**, *227*, 20-24. doi:10.1016/j.jmr.2012.11.019
43. Ernst, R. R.; Bodenhausen, G.; Wokaun, A.; *Principles of Nuclear Magnetic Resonance in One and Two Dimensions*, First Edition, Clarendon Press: Oxford, United Kingdom, 1987.
44. Le Bihan, N.; Sangwine, S. J.; Ell, T. A. Instantaneous frequency and amplitude of orthocomplex modulated signals based on quaternion Fourier transform. *Signal Processing* **2014**, *94*, 308-318. doi:10.1016/j.sigpro.2013.06.028
45. Sehgal, A. A.; Pelupessy, P.; Rolando, C.; Bodenhausen, G. Theory for spiralling ions for 2D FT-ICR and comparison with precessing magnetization vectors in 2D NMR. *Physical Chemistry Chemical Physics* **2016**, *18*(13), 9167-9175. doi:10.1039/c6cp00641h
46. Caravatti, P.; Allemann, M. The infinity cell: a new trapped-ion cell with radiofrequency covered trapping electrodes for Fourier transform ion cyclotron resonance mass spectrometry. *Org. Mass Spectrom.* **1991**, *26*(5), 514-518. doi:10.1002/oms.1210260527
47. Tsybin, Y. O.; Witt, M.; Baykut, G.; Kjeldsen, F.; Hakansson, P. Combined infrared multiphoton dissociation and electron capture dissociation with a hollow electron beam in Fourier transform ion cyclotron resonance mass spectrometry. *Rapid Commun. Mass Spectrom.* **2003**, *17*(15), 1759-1768. doi:10.1002/rcm.1118
48. Chiron, L.; Coutouly, M.-A.; Starck, J.-P.; Rolando, C.; Delsuc, M.-A. SPIKE a processing software dedicated to Fourier spectroscopies. *arXiv.org, e-Print Arch., Phys.* **2016**, 1-13. doi:arXiv:1608.06777
49. Kilgour, D. P. A.; Van Orden, S. L. Absorption mode Fourier transform mass spectrometry with no baseline correction using a novel asymmetric apodization function. *Rapid Commun. Mass Spectrom.* **2015**, *29*(11), 1009-1018. doi:10.1002/rcm.7190
50. Qi, Y.; Barrow, M. P.; Van Orden, S. L.; Thompson, C. J.; Li, H.; Perez-Hurtado, P.; O'Connor, P. B. Variation of the Fourier Transform Mass Spectra Phase Function with Experimental Parameters. *Anal. Chem.* **2011**, *83*(22), 8477-8483. doi:10.1021/ac2017585
51. O'Connor, P. B.; McLafferty, F. W. High-resolution ion isolation with the ion cyclotron resonance capacitively coupled open cell. *J. Am. Soc. Mass Spectrom.* **1995**, *6*(6), 533-535. doi:10.1016/1044-0305(95)00232-3
52. O'Connor, P. B.; Little, D. P.; McLafferty, F. W. Isotopic Assignment in Large-Molecule Mass Spectra by Fragmentation of a Selected Isotopic Peak. *Anal. Chem.* **1996**, *68*(3), 542-545. doi:10.1021/ac950599z
53. Smith, D. F.; Blakney, G. T.; Beu, S. C.; Anderson, L. C.; Weisbrod, C. R.; Hendrickson, C. L. Ultrahigh Resolution Ion Isolation by Stored Waveform Inverse Fourier Transform 21 T Fourier Transform Ion Cyclotron Resonance Mass Spectrometry. *Anal. Chem.* **2020**, *92*(4), 3213-3219. doi:10.1021/acs.analchem.9b04954
54. Thomas, M. J.; Collinge, E.; Witt, M.; Palacio Lozano, D. C.; Vane, C. H.; Moss-Hayes, V.; Barrow, M. P. Petroleomic depth profiling of Staten Island salt marsh soil: 2ω detection FTICR MS offers a new solution for the analysis of environmental contaminants. *Sci. Tot. Env.* **2019**, *662*, 852-862. doi:10.1016/j.scitotenv.2019.01.228
55. Grosshans, P. B.; Marshall, A. G. Can Fourier transform mass spectral resolution be improved by detection at harmonic multiples of the fundamental ion cyclotron orbital frequency? *Int. J. Mass Spectrom. Ion Process.* **1991**, *107*(1), 49-81. doi:10.1016/0168-1176(91)85073-U
56. Vorobyev, A.; Gorshkov, M. V.; Tsybin, Y. O. Towards data acquisition throughput increase in Fourier transform mass spectrometry of proteins using double frequency measurements. *Int. J. Mass Spectrom.* **2011**, *306*(2), 227-231. doi:10.1016/j.ijms.2010.11.020
57. Park, S.-G.; Anderson, G. A.; Bruce, J. E. Parallel Detection of Fundamental and Sixth Harmonic Signals Using an ICR Cell with Dipole and Sixth Harmonic Detectors. *J. Am. Soc. Mass Spectrom.* **2020**, *31*(3), 719-726. doi:10.1021/jasms.9b00144
58. Lam, Y. P. Y.; Wootton, C. A.; Hands-Portman, I.; Wei, J.; Chiu, C. K. C.; Romero-Canelon, I.; Lermyte, F.; Barrow, M. P.; O'Connor, P. B. Does deamidation of islet amyloid polypeptide accelerate amyloid fibril formation? *Chem. Comm.* **2018**, *54*(98), 13853-13856. doi:10.1039/C8CC06675B
59. Stensland, M.; Holm, A.; Kiehne, A.; Fleckenstein, B. Targeted analysis of protein citrullination using chemical modification and tandem mass spectrometry. *Rapid Commun. Mass Spectrom.* **2009**, *23*(17), 2754-2762. doi:10.1002/rcm.4185