

Article

Methodology for Addressing Infectious Aerosol Persistence in Real-Time Using Sensor Network

Sepehr Makhsous ^{1,*}, Joelle M. Segovia ¹, Jiayang He ¹, Daniel Chan ², Larry Lee ⁴, Igor V. Novosselov ¹ and Alexander V. Mamishev ³

¹ University of Washington, Department of Mechanical Engineering, 3900 E Stevens Way NE, Seattle, WA 98195, USA; sosper30@uw.edu (SM); jsegovia@uw.edu (JMS); jh846@uw.edu (JH); ivn@uw.edu (IVN.)

² University of Washington, School of Dentistry, 1959 NE Pacific St B-307, Seattle, WA 98195, USA; dcnchan@uw.edu (DC.)

³ University of Washington, Department of Electrical and Computer Engineering, Paul Allen Center, 185 E Stevens Way NE AE100R, Seattle, WA 98195, USA; mamishev@uw.edu (AVM.)

⁴ Pacific Industrial Hygiene, LLC, 5520 106th Ave NE, Kirkland, WA 98033, USA; pacific.ih@comcast.net (LL.)

* Correspondence: sosper30@uw.edu; Tel.: +1-206-499-4618

Abstract: Human exposure to infectious aerosols results a transmission of diseases, such as influenza, tuberculosis, and COVID-19. Most dental procedures generate a significant number of aerosolized particles, increasing transmission risk in dental settings. Since the generation of aerosols in dentistry is unavoidable, many clinics started using intervention strategies such as area-filtration units and extraoral evacuation equipment, especially under the relatively recent constraints of the pandemics. However, the effectiveness of these devices in dental operatories has not been studied. Therefore, the dental personnel's ability to position and operate such instruments efficiently is also limited. To address these challenges, we utilized a real-time sensor network for assessment of aerosol dynamics during dental restoration and cleaning procedures with and without intervention. The strategies tested during the procedures were (i) local area high-efficiency particle air (HEPA) filters and (ii) extra-oral suction device (EOSD). The study was conducted at the University of Washington School of Dentistry using a network of thirteen fixed sensors positioned within the operator and one wearable sensor worn by the dental operator. The sensor network provides time and space-resolved particulate matter (PM) data. Three-dimensional (3D) visualization informs aerosol persistence in the operator. It was found that area filters did not improve the overall aerosol concentration in dental offices significantly. An average of 16% decrease in PM concentration was observed when EOSD equipment was used during the procedures. The combination of real-time sensors and 3D visualization can provide dental personnel and facility managers with actionable feedback to effectively assess aerosol transmission in medical settings and develop evidence-based intervention strategies.

Keywords: Aerosols, dental clinics, infection control, high-volume evacuation, extra-oral suction device, particle concentration, sensor network, dispersion modeling, exposure assessment, air quality

1. Introduction

Performing dental procedures for patients infected with SARS-CoV-2 or other infectious diseases can produce long-lived aerosols containing infectious virus particles [1-5]. Due to the limitation of aerosol monitoring instruments, there is limited information on the number, size, persistence, and fate of these aerosols in medical facilities and dental offices [6]. These limited data from simulated dental treatment suggests that dental aerosols can travel more than six feet from the patient's mouth and remain suspended in the operator for up to 30 minutes, depending upon particle size. The COVID-19 pandemic highlighted that many infections could be transmitted through aerosol exposure

establishing the urgent need to monitor the environment and develop evidence-based intervention strategies.

Many infectious disease carriers can show no symptoms, making it difficult for dental practices to assess each patient's risk [7]. To help mitigate the risk of transmission, the center for disease control (CDC) recommends vacuum and filtration units be used while and immediately after patient procedures [8]. These mitigation strategies can help minimize the risk of airborne disease transmissions by removing aerosolized particles using intervention techniques such as high-efficiency particle air (HEPA) filtration units and extra-oral suction device (EOSD). Yet, there are currently limited information for how effective these interventions are and how quickly they can bring the air quality back to its original levels to ensure a safe operatory environment. If the intervention strategy fails to eliminate aerosol transmission, infectious particles can be spread via three different paths, as demonstrated in Figure 1.

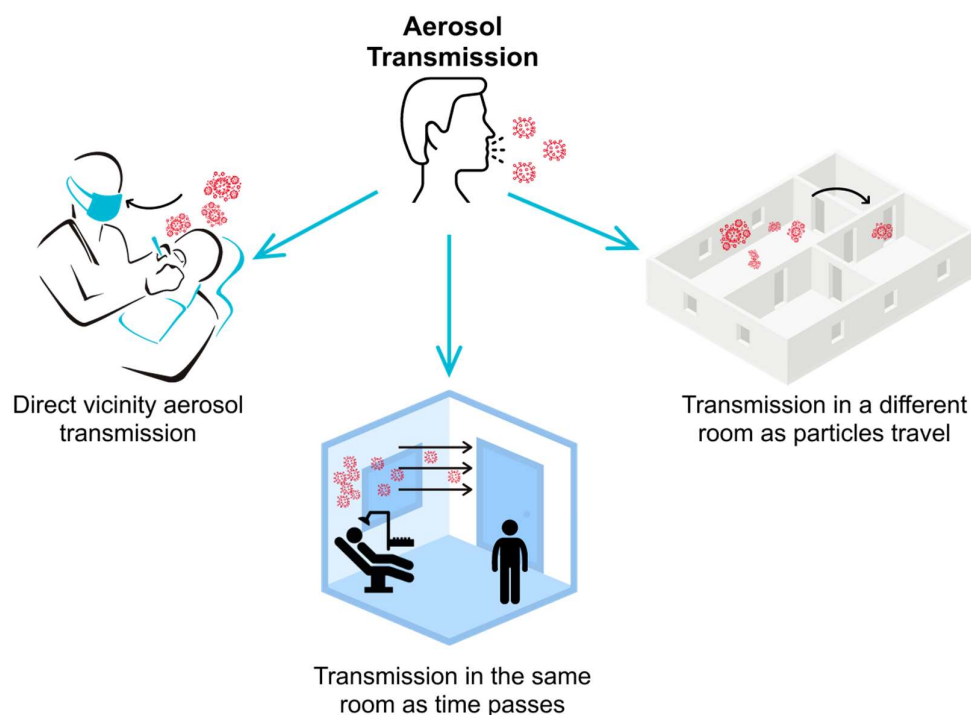


Figure 1. Aerosolized particles generated during dental operations can transmit infectious diseases via three paths: 1 - direct vicinity transmission, (dental professionals while performing high aerosol generating procedures); 2 - same room transmission as time passes, (anyone who enters the room after the procedure); and 3 - different room or location transmission, (aerosolized particles can travel to different rooms or locations in the dental office, putting everyone in those locations at risk.)

Effective aerosol monitoring should enable dental clinics to assess efficiency of the existing intervention strategies. However, professional air monitoring units can cost thousands of dollars per unit and typically available only in research labs or from air monitor consulting services. Typical reference instruments do not have networking capabilities or over air data transfer. These factors make air quality monitoring impractical for many clinics for continuous air monitoring. This paper presents a real-time, low-cost, and comprehensible air monitoring system called AeroSpec. This scalable sensor network approach utilizes Optical Particle Counters (OPCs) to gather time and space-resolved aerosol concentration and particle size distribution data. It is capable of transmitting information from individual sensor via Internet of Things (IoT) protocol, displaying the data in a custom user portal, and alerting users of high concentration levels.

Low-cost particulate matter (PM) sensors find increasing use in various applications, including monitoring AQ in the outdoor and indoor environment by academic researchers and citizen scientists. The low-cost sensor networks have the potential to provide high

spatial and temporal and resolution, identifying pollution sources and hotspots, which in turn can lead to the development of intervention strategies for exposure assessment and intervention strategies for susceptible individuals. Time-resolved exposure data from wearable monitors can be used to assess individual exposure in near real-time. Various studies have evaluated the performance of low-cost PM sensors in laboratory and field settings [9-16]; these reports show that, when calibrated against research-grade reference instruments, the low-cost sensor yield usable data, although some drawbacks have been reported.

Detectors that rely on elastic light scattering to measure time- and size-resolved PM concentrations are widely used in aerosol research, particularly when measuring particles in the 0.3 μm to 10 μm range. Low-cost sensor measurements suffer from sensor-to-sensor variability due to a lack of quality control and differences between individual components [16, 17]. Sensor geometry can be optimized to reduce the effect of particle complex index of refraction (CRI). Researchers have addressed CRI sensitivity by designing optical particle sizers (OPSs) that measure scattered light at multiple different angles simultaneously [18] or by employing dual-wavelength techniques [19]. Recently Njalsson et al. proposed optimizing the detector angle relative to excitation beam to reduce dependency on CRI [20]; however, these sensors did not enter high volume production at this time.

The low-cost sensor Plantower PMS A003 (Plantower, Beijing Ereach Technology Co., Ltd, China) was incorporated in each monitoring unit. A sensor's photodiode positioned normal to the excitation beam measures the light scattered by the particles in the optical volume. The scattering light intensity is then converted to a voltage signal to estimate PM number density and mass concentration using a proprietary calibration algorithm. The PMS provides estimated particle counts in six size bins with the optical diameter in 0.3-10 μm ($\#/0.1\text{L}$) range and mass concentration ($\mu\text{g}/\text{m}^3$) for PM_{10} , $\text{PM}_{2.5}$, and $\text{PM}_{1.0}$. In the analysis, we report time resolved total particle concentration, i.e., all particles with optical diameter greater than 0.3 μm in 0.1L of air as a function of time.

Time and space-resolved 3D aerosol monitoring requires compact instruments to provide accurate particle sizing and cost-effective operational reliability [21]. These instruments must provide data to the user in real-time, enabling corrective action based temporal and geospatial analysis. The traditional methods require laboratory-based testing methods, which cannot achieve real-time analysis. The system used in this study, AeroSpec (shown in Figure 2,) consists of compact area monitors and wearable personal exposure monitor (PEM) that incorporate PMS sensor, humidity and temperature sensors, Wi-Fi and cellular LTE chips for data transfer [22]. The data can be transmitted in real-time to the database using Wi-Fi or cellular connection. The secure digital (SD) card is used for on-board data backup. The real-time sensor data is aggregated to create a 3D map of size resolved aerosol concentration. Figure 3 demonstrates the flow diagram of the AeroSpec system and how the sensors' data-driven intervention approach can alert users of aerosol transmission routes.

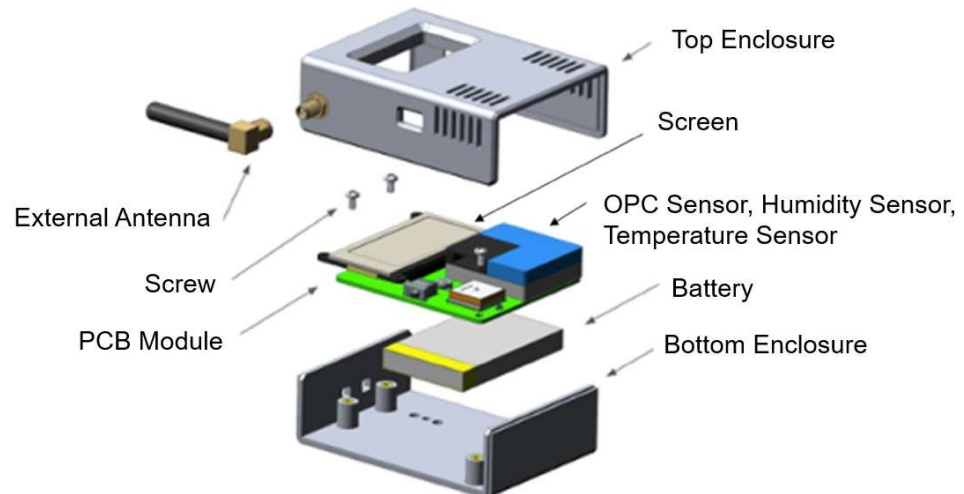


Figure 2. Exploded view of the AeroSpec hardware unit, which consists of environmental sensors, PCB board, LiPo battery, and screen. The electronics are assembled in an ABS plastic enclosure manufactured by Tool Less Plastics. The device dimensions are (H) 100 mm x (W) 60 mm x (D) 25 mm and weighs 120 g.

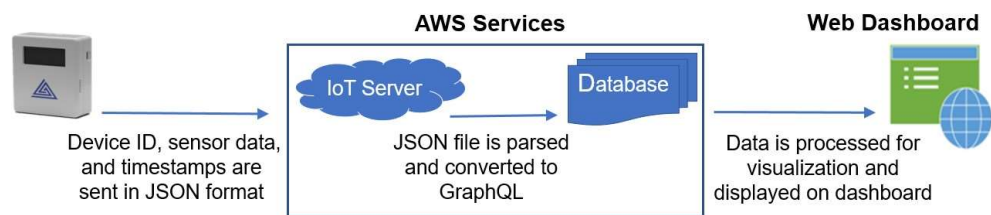


Figure 3. The AeroSpec sensor network system diagram. The hardware unit transmits the data to the AWS database as JSON format, the analyzed data is displayed in 3D visualization format on the web-based software in real-time using the AWS database.

The current methodologies have limitations in analyzing space-resolved aerosol distribution during clinical procedures. Past studies typically utilized settling plates or filter paper to collect aerosol and splatter samples [23, 24]. These studies also used dental simulation units as opposed to real patients. A study conducted at the School of Dental Sciences in Newcastle performed a crown preparation procedure on a dental simulation unit for the upper right central incisor. A full-mouth scaling procedure was done using a magnetostrictive ultrasonic scaler [25]. The methodology consisted of placing a filter paper around the immediate area and investigating the aerosol distribution and transmission routes using the photographic and spectrofluorometric analysis. It was found that the observed aerosol and splatter concentration was the highest within one and a half meters of the origin, with some aerosol readings documented as far as four meters away. The study reported that when a handheld dental suction unit is incorporated, aerosols' contamination is reduced by 75% within 0.5 and 1.5 meters of the origin.

The University of North Carolina at Chapel Hill conducted a study that evaluated the use of an extraoral suction unit (ESU) [26]. A dental manikin was used in a restorative treatment procedure. A color-changing polyvinyl chloride electrical tape grid was placed around the manikin's mouth to detect any splatter. Photo-analysis of this grid was used to determine splatter concentration and variation. Without ESU-use, 34% of the experimental grid's total surface area was found to have droplet splatter. When the ESU was set to level four out of ten-speed levels, it fell to 16% and later 8% when the ESU was set to level ten. The ESU was then set to level ten, and droplet splatter coverage was documented to have reduced to 8%. This study's findings concluded that handheld suction units are more effective in lowering aerosol distribution than the standing unit vacuums.

A study conducted by the Lublin University of Technology used optical spectrometers (OPS) units, placed inside and outside of a dental office over nine days [27]. It was found that the particle concentrations reached the highest increase during dental grinding and drilling procedures. However, there were no reports on the effectiveness of any intervention strategies used during the dental procedure.

In this paper, the AeroSpec sensor network is presented as a new methodology to measure particle concentration in dental facilities. The tests were performed at the University of Washington's School of Dentistry. The sensor network recorded time and space-resolved particulate matter concentration in real-time and produced a 3D map of particle distribution. We evaluated two most common intervention strategies, local HEPA filtration unit and EOSD device. A network of fourteen sensors was used to evaluate the EOSD device's effectiveness during high aerosolizing procedures (restoration and cleaning); as well as a network of three sensors was used to evaluate the efficiency of the HEPA filtration unit. Finally, the results from both HEPA filters and EOSD intervention strategies are outlined, along with discussing how to use the AeroSpec network to mitigate aerosol transmission in a dental setting.

2. Materials and Methods

2.1. Experimental Setup

2.1.1. Evaluating Aera Filtration Units

In assessing area filtration (HEPA) units' efficiency, sensors were placed near a Surgically Clean Air Jade air purifier to measure the particle concentration the devices emitted. Three sensors were placed in the immediate area of an isolated purifying unit in the main hallway of UW SoD. Sensor AS8 was hung approximately 60 cm above the air purifying unit's outlet fan, while sensor AS3 was placed on the floor next to the unit. The final sensor AS13 was placed on top of a trash bin next to the air purifying unit. The trash bin was taller than the air purifying unit resulting in the sensor being approximately one foot higher than the air-purifying unit's outlet fan. Figure 4 shows the sensor network set up for evaluating the HEPA filtration unit.



Figure 4. Photograph of the Surgically Clean Air Jade air purifier with three sensors (one sensor not in the field of view, located on the floor, in front of the air inlet of the filtration unit) to monitor the effects of the HEPA filter equipped air purifier.

2.1.1. Evaluating EOSD Units

To evaluate the persistence of dental aerosols during the operation and effectiveness of EOSD, fourteen AeroSpec devices were placed in an operatory located in a high-traffic educational dental clinic at different heights (shown in Figure 5). Four of the devices were placed in the hallway located between operatories C8 and D8 (shown in Figure 6). The

sensor labeled AS4 is attached close to the dentist's breathing area to measure the exact amount of personal exposure associated with different activities and dental procedures.

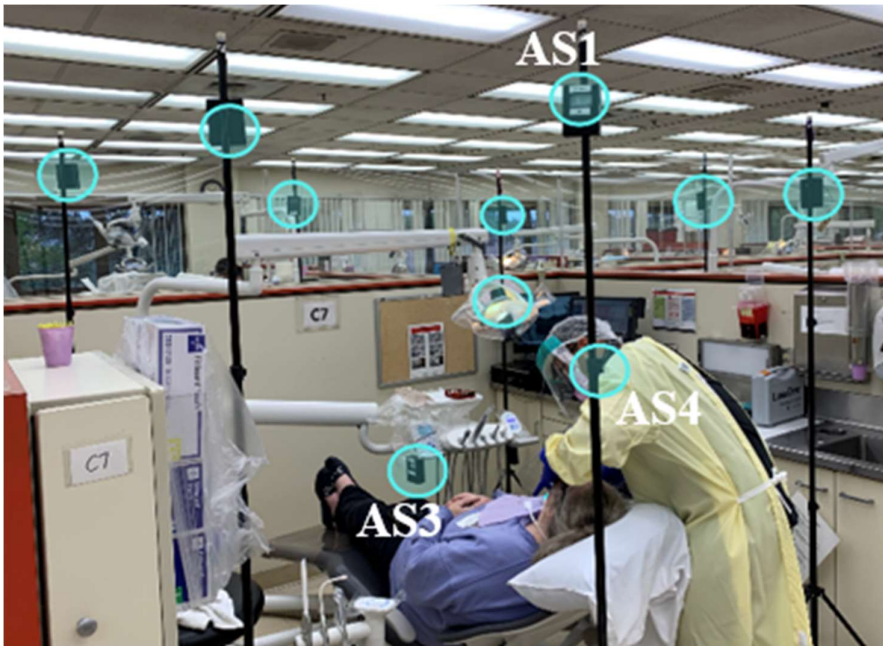


Figure 5. Photograph of the dental facility with 14 sensors (some sensors not in the field of camera view) to monitor dentists' and patients' exposure during drilling, composite removal, and cleaning operations. Sensors were placed around the operatory as well as the surrounding bays at two different heights.

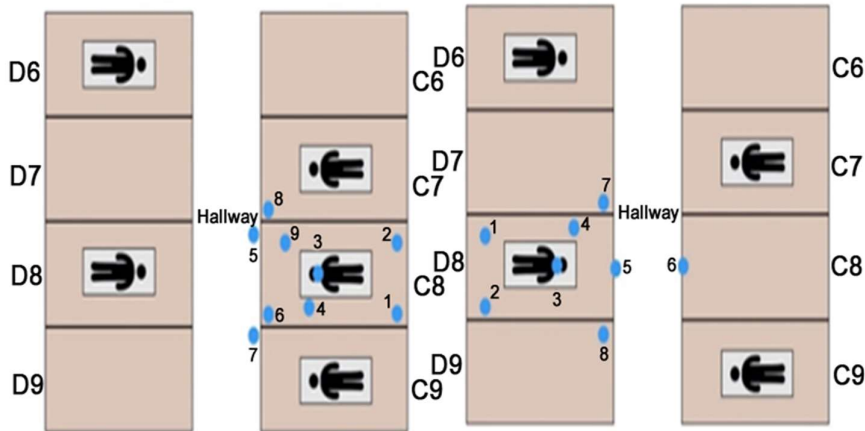


Figure 6. Positions of the sensors' network were tested in a dental operatory consisting of 16 individual bays. Two bays, C8 and D8, were equipped with the sensors.

Dentists performed regular restoration and cleaning activities while the sensor network gathered data, as shown in Figure 6. All particles greater than 0.3 μm in size were captured by the sensors and displayed every 10 seconds in real-time. Table I presents a list of events during the procedure that could have affected the area of interest. The two most effective events were Event Number Two (i.e., when the dentist began the tooth-drilling portion of the procedure) and Event Number Four (i.e., when the EOSD machine was turned to high in cubicle D8). The data collected during the cleaning procedure in cubicle C8 has been omitted due to the short window of aerosol generation available during the monitoring session.

Table I Procedures in Cubicle D8.

Event #	Time	Description
#1	2:01 PM	Cubicle D8 restoration procedure begins; Cubicle C7 has impression procedure underway.
#2 (Drilling)	2:12 PM	Cubicle D8 drilling procedure begins.
#3	2:19 PM	Cubicle C9 is cutting procedure underway.
#3a	2:31 PM	Lost connection (B17).
#4 (EOSD ON)	2:35 PM	Suction machine #1 turned on in cubicle D8 (on high mode).
#5	2:37 PM	Cubicle C8 started the examination.
#6	2:40 PM	Suction machine #1 turned off.
#6a	2:41 PM	Reset Sensor (B17).

3. Results and Discussion

The results gathered from analyzing the HEPA filter are shown in Figure 7. While the sensor placed on the floor (AS3) and the nearby trashcan (AS13) show consistent results, a drop of approximately 500 in particulate count of $Dp > 0.3$ is observed by the sensor placed next to the unit (AS8), following the fan turning on low, particle concentration doubles. Alternatively, a drop in concentration is witnessed when the fan is placed on high, and an even further reduction is observed once the fan is placed on max speed. However, the overall particle concentration reduction is minimal, caused by the unit's fan circulating the surrounding air. Upon further observation of the Surgically Clean Air Jade air purifier [28], it was noticed that the HEPA filter was not correctly sealed, causing particles to escape. As the fan's flow rate starts to increase, the particle concentration begins to drop in response due to a higher rate of dissipation.

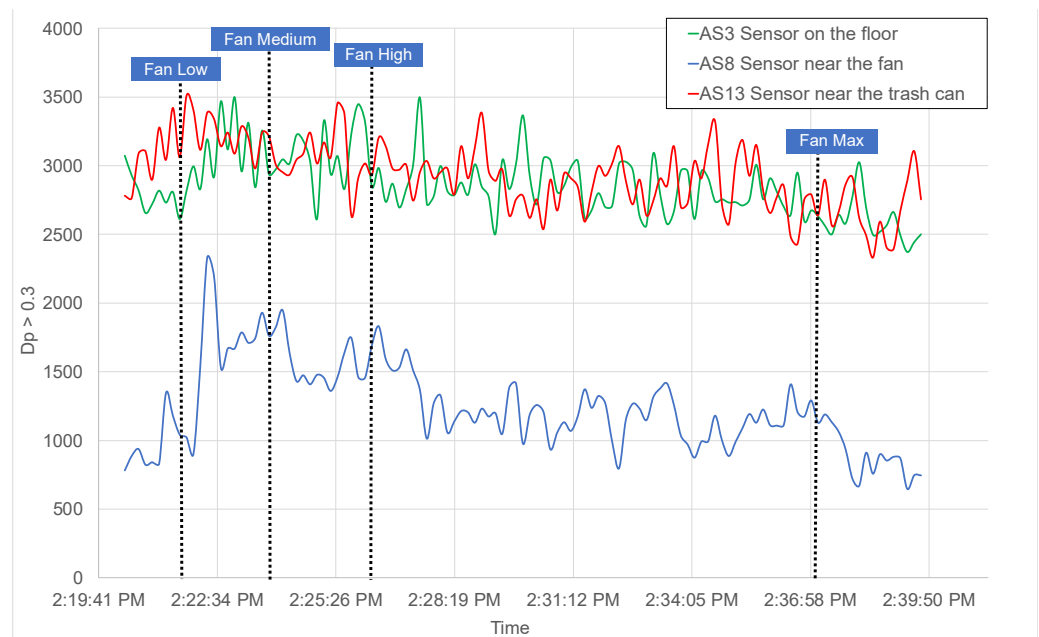


Figure 7. The number of particulates larger than PM 0.3 ($Dp > 0.3$) data from three sensors AS3, AS8, and AS13 used to evaluate the effectiveness of the Surgically Clean Air Jade HEPA air purifier is presented. The data shows a minimum change in particulate count regardless of the fan speed. After further investigation, it was discovered that the HEPA filter was not sealed properly, which caused the particles to escape and get circulated by the fan.

Figure 8 highlights the particle concentration data measured by AS4, AS3, and AS1 devices. The dental personnel wore sensor AS4. Sensor AS3 was placed closest to the patient's mouth, and AS1 was placed in the hallway. The results demonstrated the EOSD

units are not as effective around the patient's mouth and the dental personnel's breathing zone. In addition, the results in Figure 10 showed aerosolized particles travel across the hallway into the other operatories, even after new barriers were installed to separate the cubicle amid COVID-19.



Figure 8. The number of particulates larger than PM 0.3 ($D_p > 0.3$) data from three selected sensors is presented. AS4 is worn by the physician, AS3 is placed closest to the patient, and AS1 is place in the hallway outside of the dental operator bay. The spikes associated with the drilling procedure are immediately detected by AS4, putting the physician at the highest risk of transmission. Some spikes are detected by AS1, which shows that aerosolized particles are traveling across the hall and potentially contaminating other locations. The graphs are color-coded in five categories, which are defined in Figure 9.

Categories	$D_p > 0.3$ Particle Count Levels
Hazardous	> 900
Very High	800 – 900
High	700 – 800
Moderate	500 – 700
SoD Baseline	300 – 500

Figure 9. Five categories were chosen to represent different levels of exposure rate. The SoD baseline was calculated separately during active hours. The categories were defined using the same structure as PM 2.5 published by EPA [29].

The data gathered while investigating the EOSD unit showed that the drilling procedures produced an average of 465 particles with sensors AS1 (hallway), AS3 (patient), and AS4 (physician), recording an average of 427, 465, and 503 particles, respectively. For the five minutes the EOSD was run, the average particle concentration decreased to around 387 particles.

$$P_D = \sum_{t=t_i}^{t_f} P_t \quad (1)$$

where P_D is the total number of particles produced by the drilling procedure, t_i is the time when the drilling procedure started (2:12 PM), and t_f is when the procedure ended (2:35 PM). Sensor AS1 lowered to an average of 357 particles, with sensors AS3 and AS4 reporting an average of 409 and 394 particles. This shows a percentage decrease of 16.4%, 12%, and 21.5% for AS1, AS3, and AS4, respectively. The total average reduction being 16.6% in particle concentration after approximately five minutes of EOSD use

$$d = \frac{n_A - n_B}{n_B} \times 100 \quad (2)$$

where d represents percentage decrease with n_B and n_A representing the concentration before and after the EOSD was implemented, respectively in (2.)

While aerosols' average concentration was low in the observed dental operatories, personnel-based PM sensors did document high levels of individual exposure, demonstrating the need for updated intervention strategies to negate the effects of possibly harmful aerosols. Figure 10 illustrates a 3D visualization of evaluated particulate distributions at varying levels in dental practice. The addition of this visualization tactic would support new intervention strategies, such as adopting external air filtration systems at their respective optimal heights.

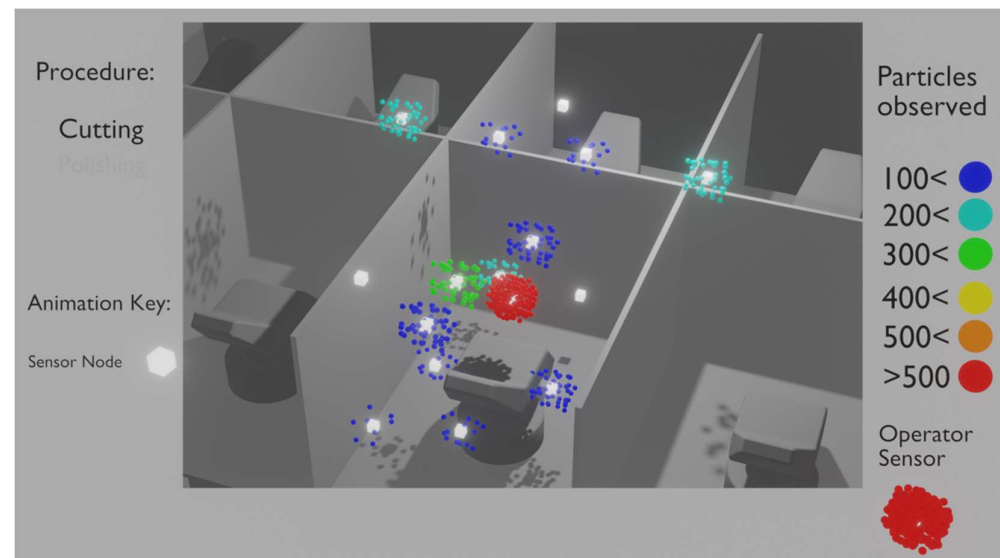


Figure 10. Real-time 3D visualization of the dental operatory D8 during a drilling procedure. Due to its importance, the operator's device is highlighted in the bottom right corner of the screen. While the aerosol concentration is at safe levels inside the cubical, the physician is being exposed to a very high concentration of aerosols.

4. Future Work

Further research will demonstrate how AeroSpec sensors monitor aerosols' generation and evaluate the effectiveness of intervention strategies used during dental procedures. This study's limitation was the short sampling time, creating a need to conduct aerosol monitoring for a more extended period of time within the dental setting.

Recording a more extended period of EOSD and air purifying units is suggested to further validate them as an existing mitigation technique. Analyzing for dead zones – areas where particles may get trapped – and areas such as waiting rooms or hallways to be monitored for high concentration can help indicate if additional areas need intervention strategies. Future studies, alongside this one, will provide the dental community with the tools necessary to determine a standardized intervention strategy to address infectious aerosol persistence in dental clinics.

5. Conclusions

The study's objective was to evaluate the effectiveness of existing aerosol distribution intervention strategies using AeroSpec monitoring systems. Current approaches applied by dental clinics lack evidence to support their efficacy in reducing aerosols. The methodology presented in this paper provides real-time aerosol distribution in 3D, which is used to determine effective interventions in the aerosol evacuation during dental procedures.

The data collected from this study found a slight reduction in particle count when EOSD units are turned on. However, the study showed that the dental personnel is at the highest risk when performing high aerosolizing procedures. In addition, an increased number of particle concentrations traveled across the hallway into other operatories, putting other patients and dental personnel at risk.

With the restrictions imposed due to the ongoing COVID-19 pandemic, the inaccuracy and drift tendencies of currently available methodologies make evaluating the efficiency of mitigation techniques challenging. Understanding how dental fields can reduce the spread of particles from high aerosol-generating procedures will further protect technicians and clients of any given facility.

Supplementary Materials: The following are available online at <https://youtu.be/tzDeGUaQHxY>, Figure 10's video: "SoD Restoration Procedure."

Author Contributions: Conceptualization, S.M. and A.V.M.; methodology, S.M. and I.V.N.; software, S.M. and J.H.; validation, S.M., J.H., and J.S.; formal analysis, S.M., J.S., I.V.N., and D.C.; investigation, S.M.; resources, D.C. and L.L.; data curation, S.M. and J.S.; writing—original draft preparation, S.M. and J.S.; writing—review and editing, S.M., I.V.N., A.V.M., L.L., and D.C.; visualization, S.M. and J.S.; supervision, S.M. and D.C.; project administration, S.M.; funding acquisition, S.M. and I.V.N.; All authors have read and agreed to the published version of the manuscript.

Funding: This research was funded by the CoMotion Director's Award from the University of Washington.

Acknowledgments: The authors thank Nhu Truong Robert A Rochlin, Nathan Hose, and Shirley Huang for their contributions to this study.

Conflicts of Interest: The authors declare no conflict of interest.

References

- [1] "Summary of ADA Guidance During the COVID-19 Pandemic." http://www.ada.org/~media/CPS/Files/COVID/COVID-19_Int_Guidance_Summary.pdf (accessed Feb. 15, 2021).
- [2] "Transmission of SARS-CoV-2: implications for infection prevention precautions," WHO Brief 2020.
- [3] J. Limeres Posse *et al.*, "The Impact of the First Wave of the COVID-19 Pandemic on Providing Special Care Dentistry: A Survey for Dentists," *International Journal of Environmental Research and Public Health*, vol. 18, no. 6, 2021, doi: 10.3390/ijerph18062970.
- [4] S. Derruau *et al.*, "COVID-19 and Dentistry in 72 Questions: An Overview of the Literature," *Journal of Clinical Medicine*, vol. 10, no. 4, 2021, doi: 10.3390/jcm10040779.
- [5] D. M. Cocârță, M. Prodana, I. Demetrescu, P. E. Lungu, and A. C. Didilescu, "Indoor Air Pollution with Fine Particles and Implications for Workers' Health in Dental Offices: A Brief Review," *Sustainability*, vol. 13, no. 2, 2021, doi: 10.3390/su13020599.

- [6] P. Han, H. Li, L. J. Walsh, and S. Ivanovski, "Splatters and Aerosols Contamination in Dental Aerosol Generating Procedures," *Applied Sciences*, vol. 11, no. 4, 2021, doi: 10.3390/app11041914.
- [7] S. Faridi *et al.*, "A field indoor air measurement of SARS-CoV-2 in the patient rooms of the largest hospital in Iran," *Science of The Total Environment*, vol. 725, p. 138401, 2020/07/10/ 2020, doi: <https://doi.org/10.1016/j.scitotenv.2020.138401>.
- [8] CDC. "Guidance for Dental Settings." CDC. <https://www.cdc.gov/coronavirus/2019-ncov/hcp/dental-settings.html> (accessed Feb. 15, 2021).
- [9] J. M. Cordero, R. Borge, and A. Narros, "Using statistical methods to carry out in field calibrations of low cost air quality sensors," *Sensors and Actuators B: Chemical*, vol. 267, pp. 245-254, 2018/08/15/ 2018, doi: <https://doi.org/10.1016/j.snb.2018.04.021>.
- [10] B. Feenstra *et al.*, "Performance evaluation of twelve low-cost PM2.5 sensors at an ambient air monitoring site," *Atmospheric Environment*, vol. 216, p. 116946, 2019/11/01/ 2019, doi: <https://doi.org/10.1016/j.atmosenv.2019.116946>.
- [11] K. E. Kelly *et al.*, "Ambient and laboratory evaluation of a low-cost particulate matter sensor," *Environmental Pollution*, vol. 221, pp. 491-500, 2017/02/01/ 2017, doi: <https://doi.org/10.1016/j.envpol.2016.12.039>.
- [12] T. Sayahi, A. Butterfield, and K. E. Kelly, "Long-term field evaluation of the Plantower PMS low-cost particulate matter sensors," *Environmental Pollution*, vol. 245, pp. 932-940, 2019/02/01/ 2019, doi: <https://doi.org/10.1016/j.envpol.2018.11.065>.
- [13] J. Tryner *et al.*, "Laboratory evaluation of low-cost PurpleAir PM monitors and in-field correction using co-located portable filter samplers," *Atmospheric Environment*, vol. 220, p. 117067, 2020/01/01/ 2020, doi: <https://doi.org/10.1016/j.atmosenv.2019.117067>.
- [14] Z. Wang, W. W. Delp, and B. C. Singer, "Performance of low-cost indoor air quality monitors for PM2.5 and PM10 from residential sources," *Building and Environment*, vol. 171, p. 106654, 2020/03/15/ 2020, doi: <https://doi.org/10.1016/j.buildenv.2020.106654>.
- [15] M. Zusman *et al.*, "Calibration of low-cost particulate matter sensors: Model development for a multi-city epidemiological study," *Environ. Int.*, vol. 134, p. 105329, 2020/01/01/ 2020, doi: <https://doi.org/10.1016/j.envint.2019.105329>.
- [16] E. Austin, I. Novosselov, E. Seto, and M. G. Yost, "Laboratory Evaluation of the Shinyei PPD42NS Low-Cost Particulate Matter Sensor," *PLOS ONE*, vol. 10, no. 9, p. e0137789, 2015, doi: 10.1371/journal.pone.0137789.
- [17] S. Sousan *et al.*, "Inter-comparison of low-cost sensors for measuring the mass concentration of occupational aerosols," *Aerosol Science and Technology*, vol. 50, no. 5, pp. 462-473, 2016/05/03 2016, doi: 10.1080/02786826.2016.1162901.
- [18] J. B. Renard *et al.*, "LOAC: a small aerosol optical counter/sizer for ground-based and balloon measurements of the size distribution and nature of atmospheric particles – Part 1: Principle of measurements and instrument evaluation," *Atmos. Meas. Tech.*, vol. 9, no. 4, pp. 1721-1742, 2016, doi: 10.5194/amt-9-1721-2016.
- [19] A. Nagy, W. W. Szymanski, P. Gál, A. Golczewski, and A. Czitrovsky, "Numerical and experimental study of the performance of the dual wavelength optical particle spectrometer (DWOPS)," *Journal of Aerosol Science*, vol. 38, no. 4, pp. 467-478, 4// 2007, doi: <http://dx.doi.org/10.1016/j.jaerosci.2007.02.005>.
- [20] T. Njalsson and I. Novosselov, "Design and Optimization of a Compact Low-cost Optical Particle Sizer," *Journal of Aerosol Science*, 2018.
- [21] L. R. Crilley *et al.*, "Evaluation of a low-cost optical particle counter (Alphasense OPC-N2) for ambient air monitoring," *Atmos. Meas. Tech.*, vol. 11, no. 2, pp. 709-720, 2018, doi: 10.5194/amt-11-709-2018.
- [22] A. Czitrovsky, "Optical Particle Counter," in *Handbook of Solid-State Lasers*, B. Denker and E. Shklovsky Eds.: Woodhead Publishing, 2013.
- [23] A. Kenarkoohi *et al.*, "Hospital indoor air quality monitoring for the detection of SARS-CoV-2 (COVID-19) virus," *Science of The Total Environment*, vol. 748, 2020, doi: 10.1016/j.scitotenv.2020.141324
- [24] J. L. Holloman, S. M. Mauriello, L. Pimenta, and R. R. Arnold, "Comparison of suction device with saliva ejector for aerosol and spatter reduction during ultrasonic scaling - The Journal of the American Dental Association," *The Journal of the American*

- Dental Association*, vol. 146, no. 1, Original Contributions Infection Control, pp. 27-33, 2021, doi: doi:10.1016/j.adaj.2014.10.001.
- [25] J. R. Allison *et al.*, "Evaluating aerosol and splatter following dental procedures: Addressing new challenges for oral health care and rehabilitation - Allison - 2021 - Journal of Oral Rehabilitation - Wiley Online Library," *Journal of Oral Rehabilitation*, vol. 48, no. 1, pp. 61-72, 2020, doi: 10.1111/joor.13098.
- [26] S. E. Chavis, S. E. Hines, D. Dyalram, W. N. Cole, and R. N. Dalby, "Can extraoral suction units minimize droplet spatter during a simulated dental procedure? - The Journal of the American Dental Association," *The Journal of the American Dental Association*, vol. 152, no. 2, pp. 157-165, 2021, doi: doi:10.1016/j.adaj.2020.10.010.
- [27] B. Polednik, "Aerosol and bioaerosol particles in a dental office," *Science Direct*, vol. 134, pp. 405-409, 2014, doi: 10.1016/j.envres.2014.06.027.
- [28] "The World's Best Indoor Air Purifiers." <https://surgicallycleanair.com/jade/> (accessed).
- [29] E. P. Agency, "Air Quality Index (AQI)," in *Air Quality Communication Workshop*, San Salvador, El Salvador, 2012. [Online]. Available: <https://www.epa.gov/sites/production/files/2014-05/documents/zell-aqi.pdf>