

Supporting Information to

Dynamic effective elasticity of melanoma cells under shear and elongational flow confirms estimation from force spectroscopy

A. M. Jötten¹, S. Neidinger¹, J.K. Tietze², J. Welzel³, C. Westerhausen^{1,4,5}

¹ Experimental Physics I, Institute of Physics, University of Augsburg, 86159 Augsburg, Germany

² Clinic and Policlinic for Dermatology and Venerology, University Medical Center Rostock, 18057 Rostock

³ Department of Dermatology, University hospital Augsburg, 86179 Augsburg, Germany

⁴ Physiology, Institute of Theoretical Medicine, University of Augsburg, 86159 Augsburg, Germany

⁵ Center for NanoScience (CeNS), Ludwig-Maximilians-Universität Munich, 80799 Munich, Germany

~ corresponding author: christoph.westerhausen@gmail.com

Young's modulus for repeated force spectroscopy on single cells

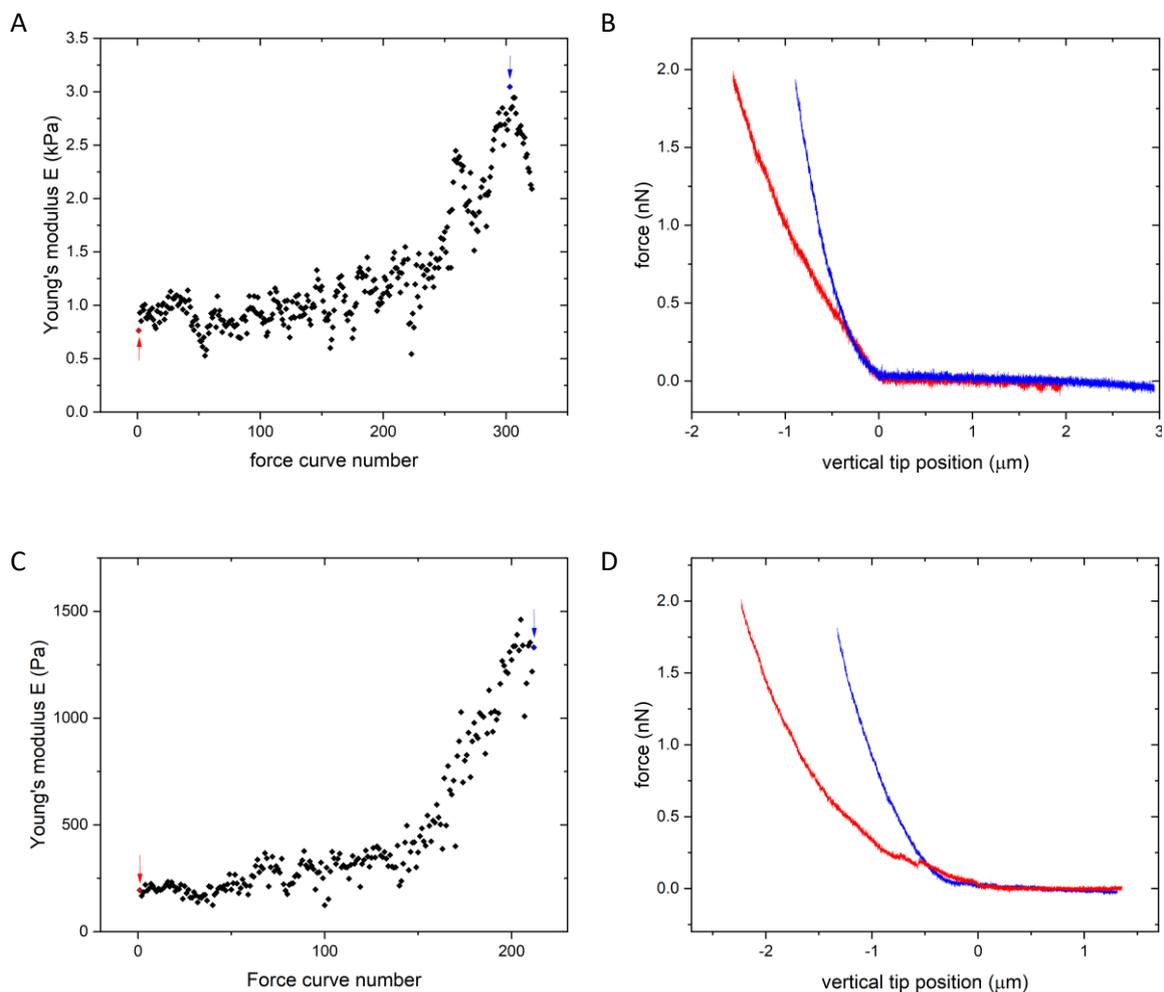


Figure S1 A) Young's modulus for repeated measurements on a single adherent A375 (cantilever MLCT-BIO with pyramidal tip, $v_{\text{approach}} = 1 \mu\text{m/s}$). B) Exemplary force distance curves for the data points highlighted in A. C) Young's modulus for repeated measurements on a single adherent A375 (independent preparation but identical conditions as in A). D) Exemplary force distance curves for the data points highlighted in C.