

## Article

# Streptavidin-Modified Iron Oxide Hybrid Nanozymes for Magnetic Enrichment and Bioelectrocatalytic Sensing of Circulating Tumor RNA

Kevin M. Koo <sup>1,2,\*</sup><sup>1</sup> The University of Queensland Centre for Clinical Research (UQCCR), QLD 4029, Australia<sup>2</sup> XING Applied Research & Assay Development (XARAD) Division, XING Technologies Pty Ltd, QLD 4073, Australia

\* Correspondence: maisheng.koo@uqconnect.edu.au

**Abstract:** Iron oxide nanozymes are a form of nanomaterial with both superparamagnetic and enzyme-mimicking properties. Given the multifunctional nature of iron oxide nanozymes, it is attractive for creating iron oxide hybrid nanozymes through biomolecular modifications to imbue with auxillary properties. Such iron oxide hybrid nanozymes can be useful for rapid and cost-effective analysis of circulating tumor nucleic acids (ctNAs) in patient liquid biopsies during minimal residual disease (MRD) monitoring of cancer recurrence. Herein, the use of streptavidin-modified iron oxide hybrid nanozymes is reported for magnetic enrichment and bioelectrocatalytic sensing of three prostate cancer (PCa) ctRNA biomarkers with high detection specificity and sensitivity (10 copies) over an ultrabroad dynamic range (five orders of magnitude). Furthermore, the feasibility of ctRNA analysis for pre- and post-cancer treatment MRD monitoring is demonstrated using PCa urinary liquid biopsy samples.

**Keywords:** nanozymes; circulating tumor nucleic acid; liquid biopsy; magnetic enrichment; minimal residual disease; cell-free RNA

## 1. Introduction

The introduction should briefly place the study in a broad context and highlight why it is important. It should define the purpose of the work and its significance. The current state of the research field should be carefully reviewed and key publications cited. Please highlight controversial and diverging hypotheses when necessary. Finally, briefly mention the main aim of the work and highlight the principal conclusions. As far as possible, please keep the introduction comprehensible to scientists outside your particular field of research. References should be numbered in order of appearance and indicated by a numeral or numerals in square brackets—e.g., [1] or [2,3], or [4–6]. See the end of the document for further details on references. Circulating tumor nucleic acids (ctNAs) are generally tumor-derived NA fragments which have been released into body fluids such as blood or urine via passive tumor cell death or active tumor cell secretion mechanisms [1,2]. As an alternative to traditional tissue biopsy procedures, ctNA detection offers unique liquid biopsy benefits of being minimally-invasive, easily obtainable, and able to provide a “complete” sampling of cancer mutations present in different parts of the tumor [3–5]. In terms of clinical applications, targeted detection of cancer-specific ctNA biomarkers has indicated the prospect of minimal residual disease (MRD) monitoring [6–10]. MRD monitoring is the continuous surveillance of cancer recurrence following primary treatment by using liquid biopsy samples to detect trace levels of ctNAs, in order to enable early management of any recurrent disease.

For effective MRD monitoring, it is paramount to have technologies that are able to accurately discriminate trace copies of ctNA biomarkers from a background of excess

wild-type NA sequences [11-13]. The most common workflow for enabling MRD monitoring is spin column-based ctNA enrichment followed by next-generation sequencing (NGS) or polymerase chain reaction (PCR) technologies for ctNA detection. However, spin column-based ctNA enrichment is time-consuming, laborious and may result in insufficient recovery and/or biased fragment size enrichment; and NGS/PCR detection technologies generally rely on the use of fluorescence labels and sophisticated readout instruments which increases assay cost and time. Hence, ctNA detection for MRD monitoring can benefit from a strategy to rapidly enrich and detect ctNA biomarkers in a cost-effective manner.

Nanozymes are nanomaterials with intrinsic enzyme-like activities and have been widely used as non-biological enzyme mimetics for biomedical applications [14-16]. Iron oxide nanoparticles have been demonstrated as peroxidase-mimicking nanozymes during electrochemical measurements [17,18]. Additionally, iron oxide nanoparticles exhibit superparamagnetic behavior at the nanoscale and are useful for magnetic enrichment of biomolecules [19-21]. Our laboratory has recently conceived a bioelectrocatalytic cycling approach which exploits magnetics to concentrate DNA as a scaffold for bringing redox-active labels into direct electrode contact for superior electrochemical signaling [22,23]. To realize rapid enrichment and cost-effective detection of ctNA at enhanced detection sensitivity during MRD monitoring, it is envisioned that a biomolecule-coupled iron oxide hybrid nanozyme can provide both magnetic enrichment and bioelectrocatalytic sensing of ctNA biomarkers from liquid biopsy samples.

Herein, the use of streptavidin-modified iron oxide hybrid nanozymes is reported for magnetic enrichment and electroanalysis of multiple ctRNA biomarkers in urinary liquid biopsy samples during MRD monitoring. Using prostate cancer (PCa) as a disease model for pre- and post-cancer treatment MRD monitoring, three PCa ctRNA urinary biomarkers [24] are magnetically enriched and subjected to an unique bioelectrocatalytic system of NA-intercalated methylene blue (MB) redox labels and streptavidin-modified iron oxide nanozymes. Furthermore, the assay is demonstrated for cost-effective usage on disposable screen-printed electrodes with zmol (10 copies) detection sensitivity and ultrabroad dynamic range over five orders of magnitude.

## 2. Results and Discussion


### 2.1. Streptavidin-Modified Iron Oxide Nanozymes for ctRNA Magnetic Enrichment and Bioelectrocatalytic Sensing

The approach of using streptavidin-modified iron oxide nanozymes for both magnetic enrichment and bioelectrocatalytic sensing of urinary ctRNA is shown in Figure 1. The detection of highly PCa-specific ctRNA biomarkers in urine has been shown to be feasible form of liquid biopsy [24]. Such ctRNA biomarkers include the gene fusion between TMPRSS2 and ERG genes (T2:ERG), and overexpression of PCA3 and KLK2.

The assay is first initiated by the direct addition of magnetic beads with silane surface chemistry to unprocessed urine samples. Under different salt conditions, ctNAs are magnetically isolated and released for rapid isothermal recombinase amplification of ctRNA biomarkers. Each biomarker is captured and amplified with biotinylated uracil bases being incorporated into the resultant amplicons on primer-modified magnetic beads. Post-isothermal amplification, streptavidin-modified iron oxide nanoparticles are added for binding to the biotinylated uracil bases within the amplicons. The superparamagnetic property of the streptavidin-modified iron oxide nanoparticles is then utilized for magnetically enriching the ctRNA biomarker amplicons on independent screen-printed electrode surfaces for bioelectrocatalysis. The use of magnetic concentration enables close contact of amplicons to the electrode surface without prior time-consuming surface modification, as well as reducing electrochemical signal variability.

To commence bioelectrocatalytic sensing, NA-intercalating MB redox labels are first added to the ctRNA biomarker amplicons on the electrode surfaces. The amplicons serve

as biological scaffolds for the intercalation of MB redox labels [22], and the streptavidin-modified iron oxide nanoparticles (incorporated within the amplicons) function as peroxidase-mimicking nanozymes to interact with MB for bioelectrocatalysis. During the bioelectrocatalytic process, intercalated MB is first reduced to leucomethylene blue (LB) with two freely diffusing electrons. The iron oxide nanozymes then served as electron sinks near the electrode surface and returned LB to oxidized MB to complete the bioelectrocatalytic process. Chronoamperometry is used to measure the current level of regenerated MB during bioelectrocatalytic sensing and the measured current is correlated to the ctRNA biomarker level.

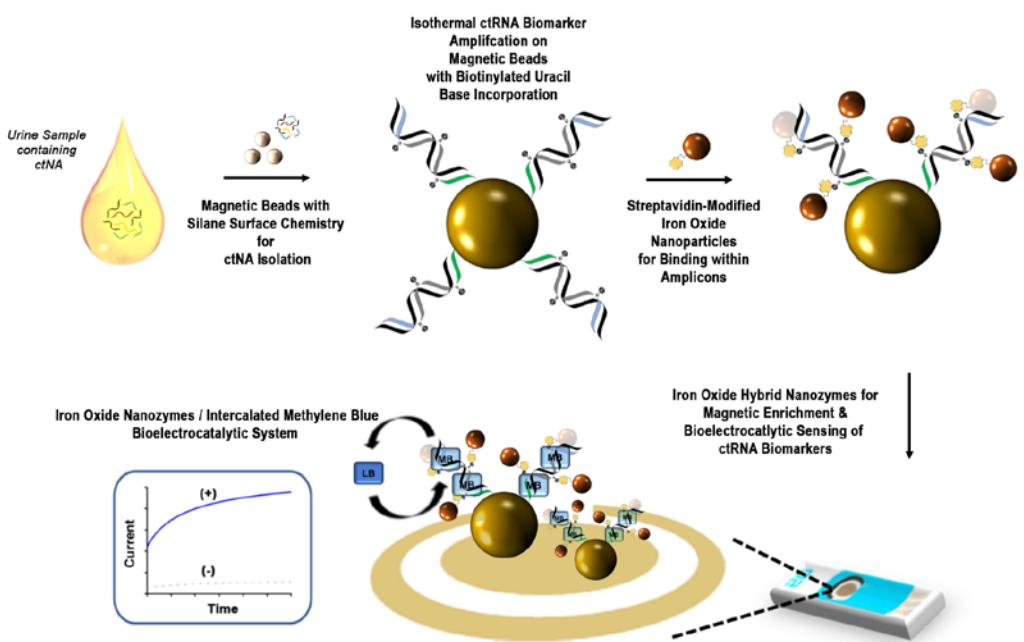

**Figure 1.** Schematic for using streptavidin-modified iron oxide nanozymes for urinary ctRNA magnetic enrichment and bioelectrocatalytic sensing.

## 2.2. Optimization of Bioelectrocatalytic Signaling Process


The bioelectrocatalytic signaling process of our assay is dependent on the amount of ctRNA biomarker amplicons being magnetically enriched on the electrode surface. The ctRNA biomarker amplicons serve as the biological scaffolds for intercalating MB redox labels and streptavidin-modified iron oxide nanozymes to generate enhanced electrochemical signaling. Thus, to achieve optimal signal enhancement, it is ideal to maximize the amount of ctRNA biomarker amplicons on the electrode surface and the signaling condition of the bioelectrocatalytic system. Therefore, parameters such as the isothermal amplification time (for producing more amplicons on the magnetic bead surface) and the pH of the electrolyte buffer (which is known to affect bioelectrocatalytic signaling kinetics) are optimized.

Firstly, different isothermal amplification times (5, 10, 15, 20, and 30 min) were tested for the producing the optimal amount of ctRNA biomarker amplicons before bioelectrocatalytic sensing. It was found that a maximal electrochemical signal was observed at 20 min and no further increase in current response change was observed thereafter (Figure S1). This was probably due to maximal coverage of ctRNA biomarker amplicons on the magnetic bead surface at 20 min during magnetic enrichment on the electrode surface, thus leading to no signal improvement beyond this timepoint. Hence, we used a 20 min isothermal amplification time for all further experiments.

Next, the electrolyte buffer pH was optimized for achieving the maximal electrochemical signal. Using different buffer pH 5.0 – 10.0, it was found that the optimal pH for generating maximal electrochemical signal occurred at pH 7.5 (Figure S2). The current level being generated improved with increased pH up to pH 7.5 but subsequently decreased thereafter. We believe that the highest signal change was obtained at pH 7.5 due to electrode surface damage lower pH, and on the contrary, the ctRNA biomarker amplicons are prone to degradation at higher pH. Hence, the electrolyte buffer pH was optimized at pH 7.5.

### 2.3. Detection Specificity for Multiple ctRNA Biomarkers

Highly specific ctRNA biomarker detection is crucial for accurate discrimination from a high background of interfering biomolecules in liquid biopsy samples. Three ctRNA biomarker-specific (T2:ERG, *PCA3*, and *KLK2*) primer pairs were designed to produce amplicons on independent sets of magnetic bead surfaces. To evaluate specific ctRNA biomarker amplification, each primer pairs were tested on various well-characterized PCa cell lines (DuCap, LnCap, 22Rv1) with known expression of T2:ERG, *PCA3*, and *KLK2*. Upon addition of paired reverse primers to initiate isothermal amplification on corresponding forward primer-modified magnetic beads, it was found that the three biomarker levels in respective PCa cell lines agreed with known expression levels (Figure 2) [17]. Thus, it was confirmed that our designed primer sets are highly specific for each of the three ctRNA biomarkers.

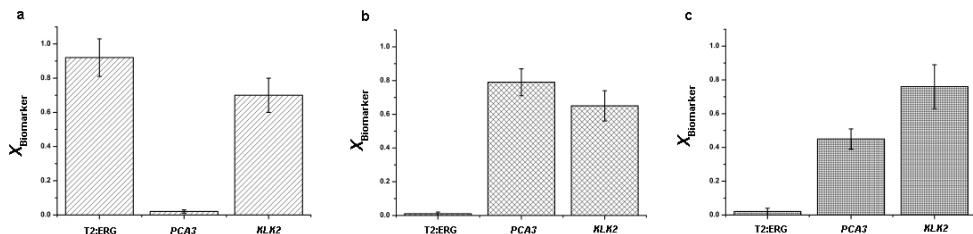


**Figure 2.** Detection of multiple ctRNA biomarkers in (a) DuCap, (b) LnCap, (c) 22Rv1 cell lines. Error bars represent standard deviations of three technical replicates.

### 2.4. Detection Sensitivity and Linear Dynamic Range

High detection sensitivity within a broad linear dynamic range is essential for trace ctRNA biomarker detection in liquid biopsy samples. To evaluate detection sensitivity and linear dynamic range, T2:ERG, *PCA3*, and *KLK2* *in vitro* transcripts over a copy number range of 0 - 1000,000 copies were evaluated for quantitative detection (Figure 3). It was observed that a clinically-relevant detection sensitivity of 10 copies was consistent across the three biomarker. The exceptional detection sensitivity was attributed to the combination of isothermal biomarker amplification, and the unique bioelectrocatalytic sensing of NA-intercalated MB redox labels and streptavidin-modified iron oxide nanzymes. In particular, the close proximity of iron oxide nanzymes and MB labels within the ctRNA biomarker amplicons is beneficial for significantly enhancing the resultant electrochemical signals. Furthermore, ultrabroad linear dynamic ranges of detection spanning over five orders of magnitude (0 – 100,000 copies) were obtained for each of the biomarkers.

In comparison to existing electrochemical assays for ctRNA detection in liquid biopsy samples [17,23,25-28], this work is distinct in utilizing streptavidin-modified iron oxide hybrid nanzymes for the dual function of magnetic enrichment and bioelectrocatalytic sensing of ctRNA biomarker amplicons. It is noteworthy that the use of streptavidin-modified iron oxide hybrid nanzymes resulted in similar assay sensitivity performance


as compared to the use of diffusive redox labels, thus highlighting the effective concept of using streptavidin to bring peroxidase-mimicking nanaozymes in close contact to MB and to the electrode surface for bioelectrocatalysis.

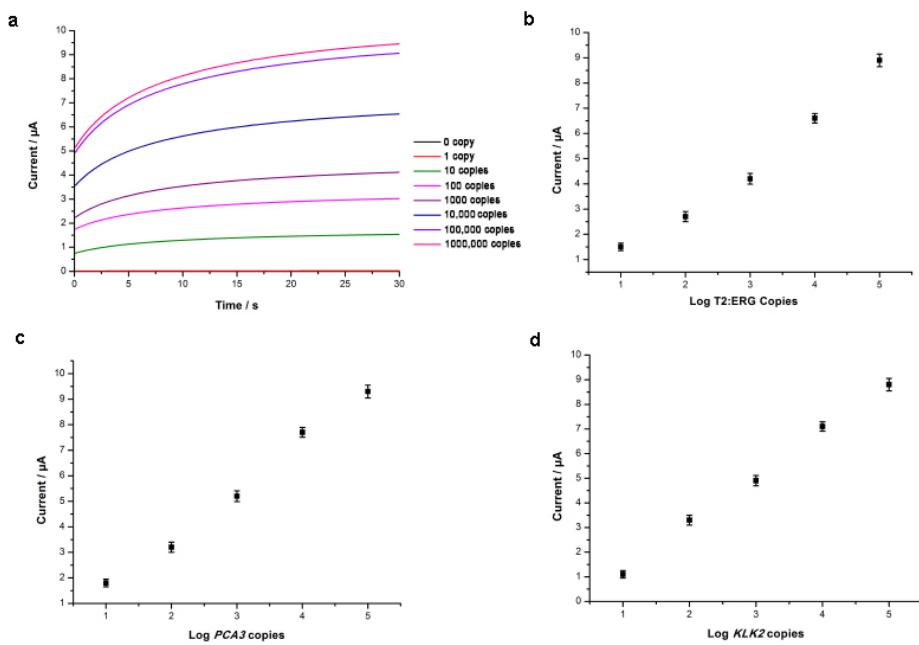

**Figure 3.** (a) Representative chronoamperometric signals for the detection of 0–1000,000 T2:ERG copies. Detection sensitivity and linear dynamic range for (b) T2:ERG, (c) PCA3, (d) KLK2. Error bars represent standard deviations of three technical replicates.

### 2.5. Minimal Residual Disease Monitoring in Patient Urine Samples for Prostate Cancer Recurrence

As a demonstration of feasibility for clinical MRD monitoring as a PCa relapse monitoring tool in urinary liquid biopsy samples. The use of urine for non-invasive MRD monitoring is beneficial for patients to be able to sequentially provide urine samples at minimal health risk and cost, especially for advanced PCa patients with non-accessible metastases such as bone-predominant lesions. To investigate the potential of avoiding serial invasive biopsies during longitudinal PCa recurrence monitoring, pre- and post-treatment urine samples of 10 PCa patients who have undergone radical prostatectomy treatment were used to perform ctRNA biomarker detection of T2:ERG, PCA3, and KLK2 (Figure 4). It was found that 4 of the 10 patients were identified with no significant decrease in T2:ERG, PCA3, and KLK2 levels after undergoing treatment, and these outcomes were correlated with diagnosed PCa biochemical recurrence. In contrary, the remaining patients displayed low gene expression of the ctRNA biomarkers and remained PCa recurrence-free. These results highlighted the feasibility of using hybrid iron oxide nanaozymes for PCa MRD monitoring from repeated liquid biopsies through the analysis of PCa-specific ctRNA biomarkers.

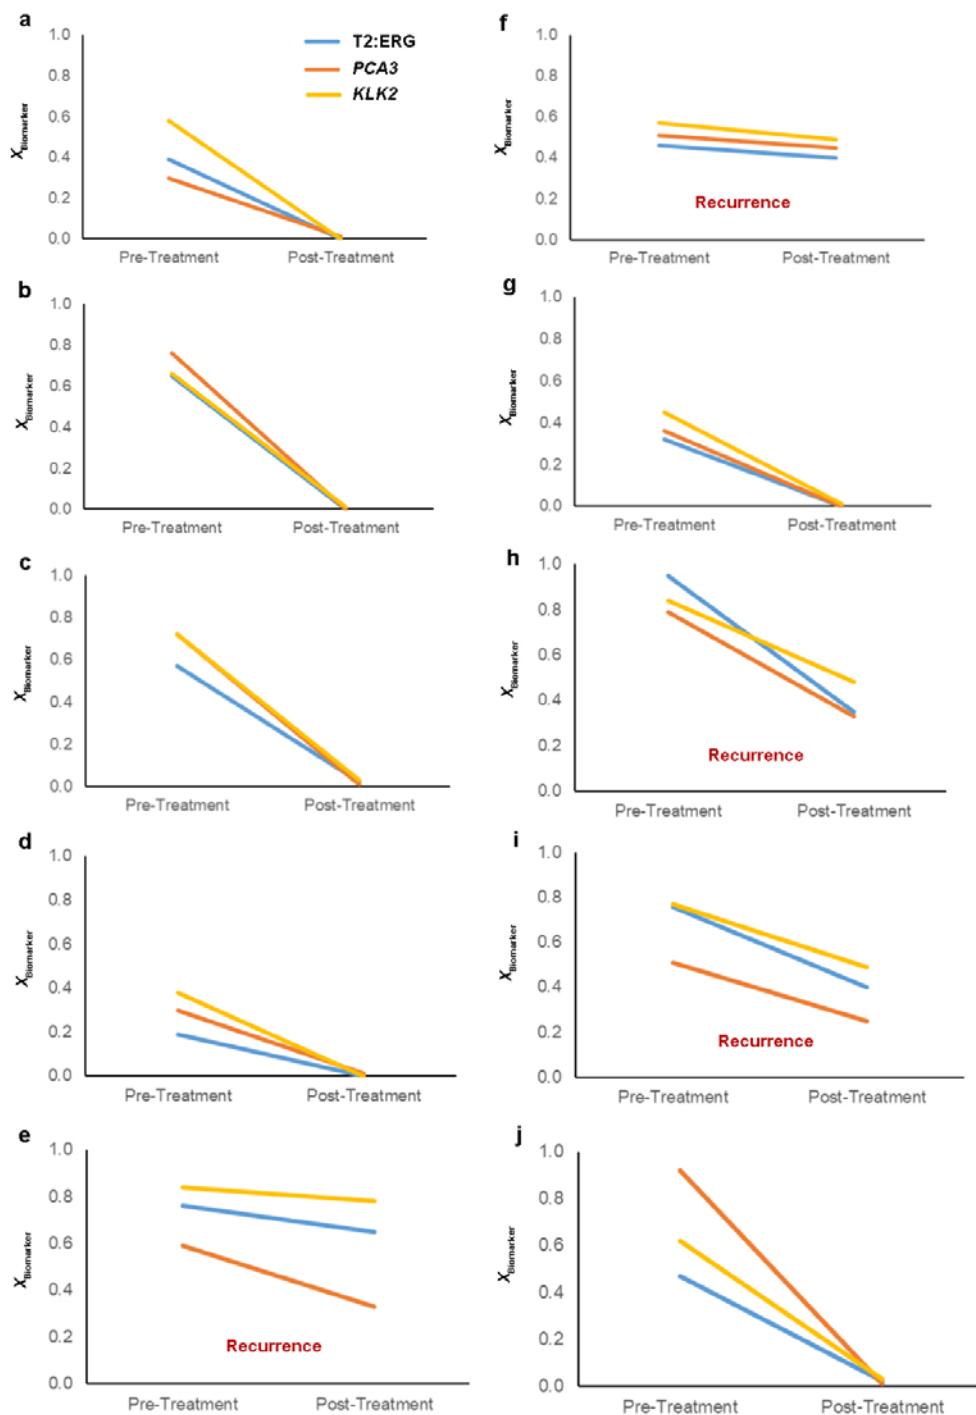

**Figure 4.** Non-invasive minimal residual disease monitoring in (a-j) pre- and post-treatment urinary liquid biopsy samples for 10 prostate cancer patients.

### 3. Materials and Methods

#### 3.1. Materials

All reagents (Sigma Aldrich) were of analytical grade and used without further purification unless otherwise stated. UltraPureTM DNase/RNase-free distilled water (Invitrogen) was used throughout the experiments. Primer sequences (Integrated DNA Technologies) used in this work are shown in Table S1.

For PCa cell lines, cells were cultured in RPMI-1640 growth media (Life Technologies) supplemented with 10% fetal bovine serum (Life Technologies) in a

humidified incubator containing 5% CO<sub>2</sub> at 37°C. For patient urine samples, ethics approval was obtained from The University of Queensland Institutional Human Research Ethics Committee (Approval No. 2004000047), and Royal Brisbane & Women's Hospital Human Research Ethics Committee (Ref No. 1995/088B). Informed consent was obtained from all subjects prior to sample collection and methods pertaining to clinical samples were carried out in accordance with approved guidelines.

### 3.2. Magnetic Isolation of ctNAs

For direct magnetic enrichment of ctNA, 1 mL of urine sample was mixed with 250 µL of Dynabead SILANE magnetic beads (Invitrogen) suspended in binding buffer (100 mM Tris-HCl, pH 7.5; 10 mM EDTA, pH 8; 500 mM LiCl; 1% LiDS; 5 mM dithiothreitol). The mixture was mixed gently to resuspend magnetic beads and then incubated for 5 min at room temperature under continuous agitation. The magnetic beads were then magnetically washed twice with 1 mL of washing buffer (10 mM Tris-HCl, pH 7.5; 1 mM EDTA; 150 mM LiCl; 0.1% LiDS). The isolated ctNA were eluted from the magnetic bead surface by incubating washed magnetic beads in 15 µL of elution buffer (10 mM Tris-HCl, pH 7.5) at 70°C for 2 min, immediately placing the mixture on a magnet, and collecting the eluted ctNA.

### 3.3. Isothermal Amplification of ctRNA Biomarkers on Magnetic Beads

Primer-functionalized magnetic beads were individually prepared for each ctRNA biomarker by incubating streptavidin-magnetic beads (10 nm, 100 µL) (Creative Diagnostics) with respective biotin-modified forward primer sequences (Table S1) on a mixer for (10 µM, 100 µL) at room temperature (30 min). After surface functionalization, excess unbound primers were removed using magnetic washing with Wash/Storage Buffer (Creative Diagnostics), and primer-functionalized magnetic beads were resuspended in UltraPure DNase/RNase-free water (200 µL). For isothermal amplification of ctRNA biomarkers, the TwistAmp Basic RT-RPA kit (Twist-DX) was used with slight modifications to manufacturer's instructions. Eluted ctNA (1.5 µL), each reverse primer (375 nM) (Table S1), biotinylated uracil bases (20 nM) (Thermo Fisher Scientific), and associated set of forward primer-functionalized magnetic beads (5 µL) were added to make a reaction volume (12.5 µL) prior to incubation (41°C, 20 min).

### 3.4. Electrochemical Detection via Iron Oxide Nanozymes/Methylene Blue Bioelectrocatalytic System

After isothermal amplification on magnetic beads, amplicons for each ctRNA biomarker were magnetically washed with Wash/Storage Buffer (Creative Diagnostics), incubated with streptavidin-modified iron oxide nanoparticles (1 µL) in phosphate buffer saline (10 mM, 0.5% triton-X pH 7.4) for 5 min to label biotinylated uracil bases, and washed again before resuspending in an electrolyte buffer (10 mM Tris, 100 mM KCl, 2.5 mM MgCl<sub>2</sub>, 1 mM CaCl<sub>2</sub>, pH 7.5) with 2 µM MB.

The resuspended mixture was dropped onto the gold working electrode surface of a DRP-C110-U75 screen-printed electrode (Metrohm), and the iron oxide nanoparticles-attached amplicons were concentrated onto the working electrode surface by positioning a permanent magnet under the electrode. Chronoamperometry measurements were carried out using a CH1040C potentiostat (CH Instruments) at -450 mV, 30 s. All measurements were performed at room temperature.

### 3.5. Data Analysis

Normalized chronoamperometric signal (X) for each ctRNA biomarker was calculated with no-template background signal taken into consideration. For example:

$$X_{T2:ERG} = (\text{raw T2:ERG signal} - \text{no-template control background signal}) / \text{no-template control background signal} \quad (1)$$

### 3.6. qPCR Validation

The KAPA SYBR® FAST One-Step qRT-PCR kit (KAPA Biosystems) was used to set up a single reaction volume for each sample (10  $\mu$ L). Each reaction volume consist of 1X KAPA SYBR® FAST qPCR Master Mix, each forward and reverse primer (200 nM) (Table S1), 1X KAPA RT Mix, ROX dye (50 nM) and eluted ctRNA (3  $\mu$ L). RT-qPCR was performed using the Applied Biosystems® 7500 Real-Time PCR System (Thermo Fisher Scientific). The cycling protocol was: 42°C for 10 min to synthesize cDNA, followed by 95°C for 5 min before cycling 40 times (95°C for 30 s, 50°C for 30 s and 72°C for 1 min) and finished with 72°C for 10 min.

## 4. Conclusions

An assay which leverages the multifunctional properties of streptavidin-modified iron oxide hybrid nanozymes was developed and demonstrated for MRD monitoring. Crucially, streptavidin-modified iron oxide nanozymes permitted rapid and cost-effective ctRNA analysis by magnetic enrichment of ctRNA biomarker amplicons on the electrode surface, and facilitated bioelectroelectrocatalytic signaling via leveraging amplicons as biological scaffolds. This rendered the assay approach more practical for PCa recurrence in urinary liquid biopsy samples by reducing analysis time and cost as compared to existing workflows. In overcoming the traditional challenges of ctRNA analysis for MRD monitoring, it is anticipated that streptavidin-modified iron oxide hybrid nanozymes may essentially be used for broad ctRNA detection applications.

**Supplementary Materials:** The following supporting information can be downloaded at xxx, Table S1: Primer sequences; Figure S1: Optimization of isothermal amplification times; Figure S2: Optimization of electrolyte buffer.

**Author Contributions:** K.M.K. conceptualized and initiated the study, performed experimental design, collected data and wrote the manuscript.

**Funding:** K.M.K acknowledges funding from the Royal Brisbane and Women's Hospital (RBWH) Foundation.

**Conflicts of Interest:** K.M.K is a scientist of XING Technologies Pty Ltd, which has licensed intellectual property from The University of Queensland.

## References

1. Rostami, A.; Lambie, M.; Yu, C.W.; Stambolic, V.; Waldron, J.N.; Bratman, S.V. Senescence, Necrosis, and Apoptosis Govern Circulating Cell-Free DNA Release Kinetics. *Cell Rep.* **2020**, *31*, 107830.
2. Heitzer, E.; Auinger, L.; Speicher, M.R. Cell-Free DNA and Apoptosis: How Dead Cells Inform About the Living. *Trends Mol. Med.* **2020**, *26*, 519-528.
3. Wan, J.C.M.; Massie, C.; Garcia-Corbacho, J.; Mouliere, F.; Brenton, J.D.; Caldas, C.; Pacey, S.; Baird, R.; Rosenfeld, N. Liquid Biopsies Come of Age: Towards Implementation of Circulating Tumour DNA. *Nat. Rev. Cancer* **2017**, *17*, 223-238.
4. Sanz-Garcia, E.; Zhao, E.; Bratman, S.V.; Siu, L.L. Monitoring and Adapting Cancer Treatment using Circulating Tumor DNA Kinetics: Current Research, Opportunities, and Challenges. *Sci. Adv.* **2022**, *8*, eabi8618.
5. Cescon, D.W.; Bratman, S.V.; Chan, S.M.; Siu, L.L. Circulating Tumor DNA and Liquid Biopsy in Oncology. *Nat. Cancer* **2020**, *1*, 276-290.
6. Kasi, P.M.; Fehringer, G.; Taniguchi, H.; Starling, N.; Nakamura, Y.; Kotani, D.; Powles, T.; Li, B.T.; Pusztai, L.; Aushev, V.N.; et al. Impact of Circulating Tumor DNA-Based Detection of Molecular Residual Disease on the Conduct and Design of Clinical Trials for Solid Tumors. *JCO Precis. Oncol.* **2022**, *6*, e2100181.
7. Garcia-Murillas, I.; Schiavon, G.; Weigelt, B.; Ng, C.; Hrebien, S.; Cutts, R.J.; Cheang, M.; Osin, P.; Nerurkar, A.; Kozarewa, I.; et al. Mutation Tracking in Circulating Tumor DNA Predicts Relapse in Early Breast Cancer. *Sci. Transl. Med.* **2015**, *7*, 302ra133.
8. Parsons, H.A.; Rhoades, J.; Reed, S.C.; Gydush, G.; Ram, P.; Exman, P.; Xiong, K.; Lo, C.C.; Li, T.; Fleharty, M.; et al. Sensitive Detection of Minimal Residual Disease in Patients Treated for Early-Stage Breast Cancer. *Clin. Cancer Res.* **2020**, 2556-2564.

9. Tie, J.; Wang, Y.X.; Tomasetti, C.; Li, L.; Springer, S.; Kinde, I.; Silliman, N.; Tacey, M.; Wong, H.L.; Christie, M.; et al. Circulating Tumor DNA Analysis Detects Minimal Residual Disease and Predicts Recurrence In Patients With Stage II Colon Cancer. *Sci. Transl. Med.* **2016**, *8*, 346ra92.

10. Einstein, D.J.; Liang, N.; Malhotra, M.; Aleshin, A.; Moshkevich, S.; Billings, P.R.; Pectasides, E. Assessment of Molecular Remission in Oligometastatic Esophageal Cancer with a Personalized Circulating Tumor DNA Assay. *JCO Precis. Oncol.* **2020**, 239-243.

11. Zeng, Y.; Koo, K.M.; Shen, A.G.; Hu, J.M.; Trau, M. Nucleic Acid Hybridization-Based Noise Suppression for Ultraselective Multiplexed Amplification of Mutant Variants. *Small* **2021**, *17*, e2006370.

12. Newman, A.M.; Lovejoy, A.F.; Klass, D.M.; Kurtz, D.M.; Chabon, J.J.; Scherer, F.; Stehr, H.; Liu, C.L.; Bratman, S.V.; Say, C.; et al. Integrated Digital Error Suppression for Improved Detection of Circulating Tumor DNA. *Nat. Biotechnol.* **2016**, *34*, 547-555.

13. Wu, L.R.; Chen, S.X.; Wu, Y.; Patel, A.A.; Zhang, D.Y. Multiplexed Enrichment of Rare DNA Variants via Sequence-Selective and Temperature-Robust Amplification. *Nat. Biomed. Eng.* **2017**, *1*, 714-723.

14. Koo, K.M.; Carrascosa, L.G.; Trau, M. DNA-Directed Assembly of Copper Nanoblocks with Inbuilt Fluorescent and Electrochemical Properties: Application in Simultaneous Amplification-Free Analysis of Multiple RNA Species. *Nano Res.* **2017**, *11*, 940-952.

15. Li, J.; Koo, K.M.; Wang, Y.; Trau, M. Native MicroRNA Targets Trigger Self-Assembly of Nanozyme-Patterned Hollowed Nanocuboids with Optimal Interparticle Gaps for Plasmonic-Activated Cancer Detection. *Small* **2019**, *15*, e1904689.

16. Wu, J.; Wang, X.; Wang, Q.; Lou, Z.; Li, S.; Zhu, Y.; Qin, L.; Wei, H. Nanomaterials with Enzyme-Like Characteristics (Nanozymes): Next-Generation Artificial Enzymes (II). *Chem. Soc. Rev.* **2019**, *48*, 1004-1076.

17. Koo, K.M.; Dey, S.; Trau, M. A Sample-to-Targeted Gene Analysis Biochip for Nanofluidic Manipulation of Solid-Phase Circulating Tumor Nucleic Acid Amplification in Liquid Biopsies. *ACS Sensors* **2018**, *3*, 2597-2603.

18. Gao, L.Z.; Zhuang, J.; Nie, L.; Zhang, J.B.; Zhang, Y.; Gu, N.; Wang, T.H.; Feng, J.; Yang, D.L.; Perrett, S.; et al. Intrinsic Peroxidase-Like Activity of Ferromagnetic Nanoparticles. *Nat. Nanotechnol.* **2007**, *2*, 577-583.

19. Koo, K.M.; Soda, N.; Shiddiky, M.J.A. Magnetic Nanomaterial-Based Electrochemical Biosensors for the Detection of Diverse Circulating Cancer Biomarkers. *Curr. Opin. Electrochem.* **2021**, *25*, 100645.

20. Soda, N.; Gonzaga, Z.J.; Chen, S.; Koo, K.M.; Nguyen, N.-T.; Shiddiky, M.J.A.; Rehm, B.H.A. Bioengineered Polymer Nanobeads for Isolation and Electrochemical Detection of Cancer Biomarkers. *ACS Appl. Mater. Interfaces* **2021**, *13*, 31418-31430.

21. Chen, H.-W.; Fang, Z.-S.; Chen, Y.-T.; Chen, Y.-I.; Yao, B.-Y.; Cheng, J.-Y.; Chien, C.-Y.; Chang, Y.-C.; Hu, C.-M.J. Targeting and Enrichment of Viral Pathogen by Cell Membrane Cloaked Magnetic Nanoparticles for Enhanced Detection. *ACS Appl. Mater. Interfaces* **2017**, *9*, 39953-39961.

22. Koo, K.M.; Trau, M. Direct Enhanced Detection of Multiple Circulating Tumor DNA Variants in Unprocessed Plasma by Magnetic-Assisted Bioelectrocatalytic Cycling. *ACS Sens.* **2020**, *5*, 3217-3225.

23. Koo, K.M.; Trau, M. Molecular Locker Probe Enrichment of Gene Fusion Variants from Matched Patient Liquid Biopsy Specimens for Magneto-Bioelectrocatalytic Nanosensing. *Nanoscale* **2022**, *14*, 4225-4233.

24. Koo, K.M.; Mainwaring, P.N.; Tomlins, S.A.; Trau, M. Merging New-Age Biomarkers and Nanodiagnostics for Precision Prostate Cancer Management. *Nat Rev. Urol.* **2019**, *16*, 302-317.

25. Koo, K.M.; Carrascosa, L.G.; Shiddiky, M.J.A.; Trau, M. Amplification-Free Detection of Gene Fusions in Prostate Cancer Urinary Samples Using mRNA-Gold Affinity Interactions. *Anal. Chem.* **2016**, *88*, 6781-6788.

26. Wen, Q.; Liang, X.; Pan, H.; Li, J.; Zhang, Y.; Zhu, W.; Long, Z. Rapid and Sensitive Electrochemical Detection of MicroRNAs by Gold Nanoparticle-Catalyzed Silver Enhancement. *Analyst* **2020**, *145*, 7893-7897.

27. Zhou, H.; Zhang, J.; Li, B.; Liu, J.; Xu, J.-J.; Chen, H.-Y. Dual-Mode SERS and Electrochemical Detection of miRNA Based on Popcorn-like Gold Nanofilms and Toehold-Mediated Strand Displacement Amplification Reaction. *Anal. Chem.* **2021**, *93*, 6120-6127.

28. Koo, K.M.; Dey, S.; Trau, M. Amplification-Free Multi-RNA-Type Profiling for Cancer Risk Stratification via Alternating Current Electrohydrodynamic Nanomixing. *Small* **2018**, *14*, 1704025.