

## Article

# Dispersion of Airborne Nanoparticles in a Gas-Liquid Dual-Microchannel Separated by a Porous Membrane: A Numerical Study

Zohreh Sheidaei<sup>1,2</sup>, Pooria Akbarzadeh<sup>1,\*</sup>, Carlotta Guiducci<sup>2</sup> and Navid Kashaninejad<sup>3,\*</sup>

<sup>1</sup> Faculty of Mechanical and Mechatronics Engineering, Shahrood University of Technology, Iran; akbarzad@ut.ac.ir

<sup>2</sup> Laboratory of Life Sciences Electronics, École Polytechnique Fédérale de Lausanne, 1015 Lausanne, Switzerland; zohreh.sheidaei@epfl.ch; carlotta.guiducci@epfl.ch

<sup>3</sup> Queensland Micro- and Nanotechnology Centre, Nathan Campus, Griffith University, 170 Kessels Road, Brisbane, QLD 4111, Australia; n.kashaninejad@griffith.edu.au


\* Correspondence: akbarzad@ut.ac.ir (P.A.); p.akbarzadeh@shahroodut.ac.ir (P.A.); Tel.: +989122022776; n.kashaninejad@griffith.edu.au (N.K.); Tel.: +61737355391

**Abstract:** Recently, there has been increasing attention toward inhaled nanoparticles (NPs) to develop inhalation therapies for diseases associated with the pulmonary system and investigate the toxic effects of hazardous environmental particles on human lung health. Taking advantage of microfluidic technology for cell culture applications, lung-on-a-chip devices with great potential in replicating the lung air-blood barrier (ABB) have opened new research insights in preclinical pathology and therapeutic studies associated with aerosol NPs. Surprisingly, the air interface in such devices, which makes them tremendously unique among the other common liquid-based cellular microsystems and enables exposure of cultivated cells to the drug/toxic aerosols, has been largely disregarded. Accordingly, there exists a significant research gap in the comprehensive understanding of the NPs' dynamics in the lung-on-a-chip devices, which is momentous to controlling the injection of aerosols to the target area and attaining the desired physiochemical efficacy. To address this research gap, a numerical parametric study is presented to provide a deep insight into the dynamic behavior of the airborne NPs in a gas-liquid dual-channel lung-on-a-chip device with a porous membrane separating the channels. A finite element multi-physics model is developed to enable a particle tracing investigation simultaneously in both air and medium phases to replicate the *in vivo* conditions avoiding laborious and costly experimental trials. The results include the impact of fluid flow as well as geometrical properties on the distribution, deposition, and translocation of the NPs with diameters ranging from 10 nm to 900 nm in the lung-on-a-chip. The obtained results strongly suggest the aerosol injection of NPs instead of the aqueous solution for more efficient deposition on the substrate of the air channel and higher translocation to the media channel. Comparative studies against accessible data as well as an experimental study are conducted to establish the accuracy of the present numerical analysis. The current study proposes to optimize the affecting parameters to control the injection and delivery of aerosol particles into the lung-on-chip device depending on the objectives of biomedical investigations and provides optimized values for some specific cases. Therefore, this study can assist scientists and researchers in complementing their experimental investigation in future preclinical studies on pulmonary pathology associated with inhaled hazardous and toxic environmental particles, as well as therapeutic studies for developing inhalation drug delivery.

**Keywords:** lung-on-a-chip; porous membrane; gas-liquid dual-channel chip; nanoparticle; numerical simulation

## 1. Introduction

As a main component of the lungs, alveoli, with a sizeable capillary interface, enable mass transfer and gas exchange in human body through their **air-blood barrier (ABB)** (see Figure 1a) [1]. They are consistently exposed to various inhaled NPs, which due to their small size, can easily transfer throughout the airways and reach there. Some NPs deposit on the alveolar epithelial cells, while others tend to cross the high-permeable ABB and transfer toward other organs and tissues through the vascular system [2,3,4]. Over the last decades, morbidity statistics have demonstrated a generous increase in severe pulmonary disorders, including asthma, emphysema, chronic obstructive pulmonary disease, and lung cancer, and highlighted inhaled exposure of alveoli to ambient toxic NPs as the main cause [5,6]. Moreover, now evidence unexpectedly reveals a growing list of other extrapulmonary diseases associated with the translocation of inhaled toxin NPs from the alveoli to the other organs such as brain, kidney, and liver [7]. On the other hand, this transfer mechanism has been recently taken into account in inhalation therapies to develop inhaled nano-drug delivery systems as a targeted and noninvasive method with fewer side effects for the treatment of pulmonary and even other organs' diseases [5]. Therefore, all of this results in a burgeoning demand for pathology, toxicology, and therapeutical studies linked with the inhaled NPs in the alveolar region in order to assess the adverse and beneficial effects of inhaled NPs on the target organ or tissue.

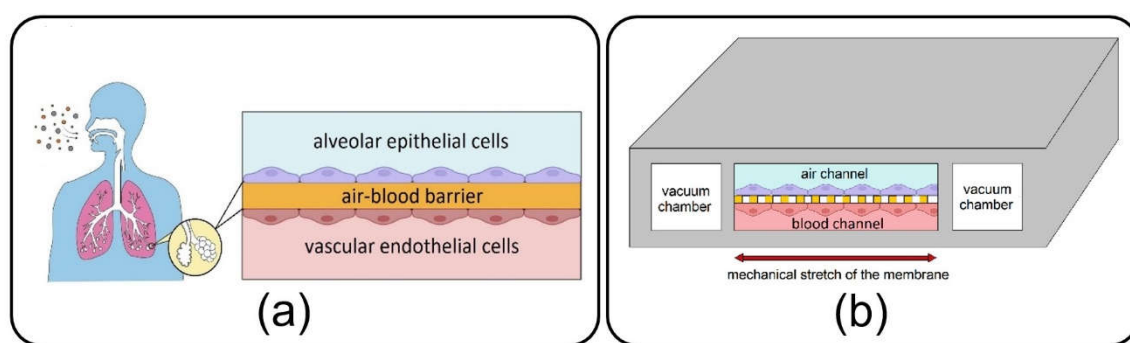

**Figure 1.** (a) Air-blood barrier (ABB) in the alveolar space of human lungs; (b) Microfluidic lung-on-a-chip device comprises air/blood channels separated by a thin, porous membrane and two side vacuum channels.

Microfluidic lung-on-a-chip device has recently drawn attention in biomedical studies owing to its unique potential in biomimicking the physiology of the lung alveolar ABB and providing more accuracy in cellular responses as compared to conventional cell culture models. First introduced by Huh et al. [8] in 2010, the lung-on-a-chip comprises air/blood (alveolar/vascular) microchannels separated by a thin porous membrane to enable the co-culturing of epithelial and endothelial cells neighboring on the opposite sides of the membrane and two side vacuum chambers to emulate a breathing lung (see Figure 1b). Advantageously, this device has opened new research doors in toxico-pharmacological fields in addition to promising an enormous capacity in recapitulating complex biological pulmonary malfunctions, such as edema formation and thrombosis [9,10]. Lung-on-a-chip devices could be conveniently utilized to inject toxic and medical aerosol NPs to replicate inhaled delivery into the alveoli for pathological and therapeutic studies, avoiding unnecessary clinical trials and animal tests. While the air interface in the lung-on-a-chip makes it tremendously unique among the other common liquid-based cellular microsystems, most of the relevant experimental studies aim at streaming an aqueous solution of NPs [8,11,12], and exposure of cultivated cells to the aerosols has been disregarded. Controlled injection of NPs into the lung-on-a-chip will return appropriate sedimentation and distribution in the target area, which is momentous to attain the desired physiochemical efficacy. However, a big research gap exists in the comprehensive understanding of the dynamics of NPs in the lung-on-a-chip device. Accordingly, the

distribution and deposition of particles on the endothelial cells in the air channel as well as their translocation to the media channel, are imperative subjects that should be examined carefully. It is evident that the dynamic behavior of particles in microdevices is impressed by many crucial factors, such as the geometry of the device and properties of fluid flow and particles. Nevertheless, optimizing all these parameters is challenging for an enhanced delivery process. Complications associated with fabricating the lung-on-a-chip device and especially the membrane with micro-scale pores, aerosol delivery, and transient monitoring of NPs, which consequently lead to costly and laborious optimization procedures, are the prime suspects responsible for such deficiencies in the field [13–15].

Many efforts have been directed toward employing numerical approaches to overcome challenges associated with experimental analyses of various cell-based microfluidic devices to improve their functionality [16,17]. A few recent investigations are devoted to studying the dynamic behavior of solid particles in the lung-on-a-chip. According to their research objectives, these studies follow two main perspectives; Namely, the Eulerian approach, which focuses on the concentration of particles considering the problem governed by typical convection-diffusion phenomena, and the Lagrangian approach that deals with individual particles, tracing the trajectory of each particle separately. For instance, Frost et al. [18] numerically investigated the effect of a porous membrane, modeled by molecular diffusivity, on the molecular convection-diffusion transport in a bilayer microfluidic device. Their results showed that the molecular concentration at the outlet of the bottom channel increased by membrane porosity augmentation, while it was invertedly affected by the upper channel height.

Although molecule-sized particles are widely considered in many biomedical studies because of their simple diffusivity, particular attention has also been recently paid to particles with diameters ranging between 10 nm to 10  $\mu\text{m}$  due to some other advantages, such as high uptake capacity by cells [19,20]. Because the Eulerian method investigates the average behavior of particles with less computational cost, it is often favored over its more precise counterpart, i.e., the Lagrangian approach. However, the outcome of these two perspectives would not converge for investigating large particles' dynamics, especially when the total number of released particles is relatively low [21]. Using the Lagrangian approach, Arefi et al. [22] studied the deposition of NPs in an air microchannel under a pulsatile bidirectional flow to simulate breathing patterns. They revealed that increased airflow rate and breathing frequency raise the deposition rate of particles on the substrate of the channel. In another similar study using finite element simulation, Moghadas et al. [23] reported that airborne delivery of NPs to the cellular region in a microchannel is affected by airflow velocity as well as particle diameter.

The lung-on-a-chip device, which enables particle tracing in air and media phases, allows for simultaneously investigating the particles' deposition and translocation. Thus, it is an essential prerequisite for precise toxicological and pharmaceutical studies. Despite its great potential in mimicking the *in vivo* conditions, the dynamics of NPs in a typical lung-on-a-chip device with a porous membrane and air/blood channels have never been investigated, to the best of our knowledge. To bridge this research gap, the current paper aims to conduct a comprehensive numerical parametric study to provide a clear insight into the role of various hydrodynamical and geometrical properties on the dynamics of airborne NPs in the lung-on-a-chip system. The impact of fluid-flow velocity, membrane porosity and particle diameter, as dominant factors, is examined on the dispersion of the particles in both air and media channels as well as their deposition and transfer rates.

This paper is organized as follows: the numerical modeling of the lung-on-a-chip, the governing equations, and boundary conditions are introduced in Section 2; comparative studies against accessible data and an experimental study are conducted in Section 3 to establish the accuracy of the present numerical study; a case study and parameter sensitivity are discussed in Section 4; and finally, Section 5 provides the conclusions and summarizes the results.

## 2. Governing Equations and Boundary Conditions

In the current work, the dynamics of airborne NPs in the gas/liquid (air/blood) channels of a lung-on-a-chip device separated by a thin, porous membrane are investigated against variations in fluid flow velocity, membrane porosity, and particle diameter. For this purpose, a 2D numerical model is developed using Laminar Flow and Particle Tracing for Fluid Flow modules in COMSOL Multiphysics 5.6 finite element software (see Figure 2) [24] to trace the motion of NPs. For simplicity, the system of governing equations is assumed to be one-way coupled, considering only the effect of the fluid regime on particles and ignoring the reactive effect due to the tiny size of particles. Therefore, first, the time-dependent velocity profile of the fluids is calculated in the channels, and then the obtained solutions are employed to solve the particle tracing. Here, it should be noted that small dimensions and low fluid velocity generally result in laminar fluid flow in microchannels and also allow the airflow to be treated as an incompressible fluid. Moreover, with a Knudsen number smaller than the critical value ( $Kn < 0.01$ ), the continuum hypothesis and no-slip velocity condition are valid for the airflow field in the channel [25]. The Knudsen number is calculated as follows:

$$Kn = \frac{\lambda}{l} = \frac{k_B}{\sqrt{2}\pi d_p^2 \rho R l}, \quad (1)$$


where  $\lambda$  is the mean free path and  $l$  is the length.  $d_p$  demonstrates the particle diameter,  $R$  and  $\rho$  represent the specific gas constant (for air is 287.05 J/(kg.K)) and fluid density, and  $k_B$  is Boltzmann constant.

In many experimental studies, blood flow is mainly replaced by a medium flow to supply the cells with required nutrition in microfluidic devices, which could be conveniently considered as a Newtonian fluid with similar hydrodynamic properties of water at 37°C [23]. Consequently, the Newtonian and incompressible air and medium phases are governed by continuity and momentum equations as follows [26]:

$$\nabla \cdot u_i = 0, \quad (2)$$

$$\rho_i \left( \frac{\partial u_i}{\partial t} + u_i \cdot \nabla u_i \right) = -\nabla p_i + \mu_i \nabla^2 u_i + \rho_i g, \quad (3)$$

where  $u$  and  $p$  represent the fluid velocity field and pressure, and  $t$  is the time, while the subscript ( $i = a, m$ ) stands for air and media, respectively.

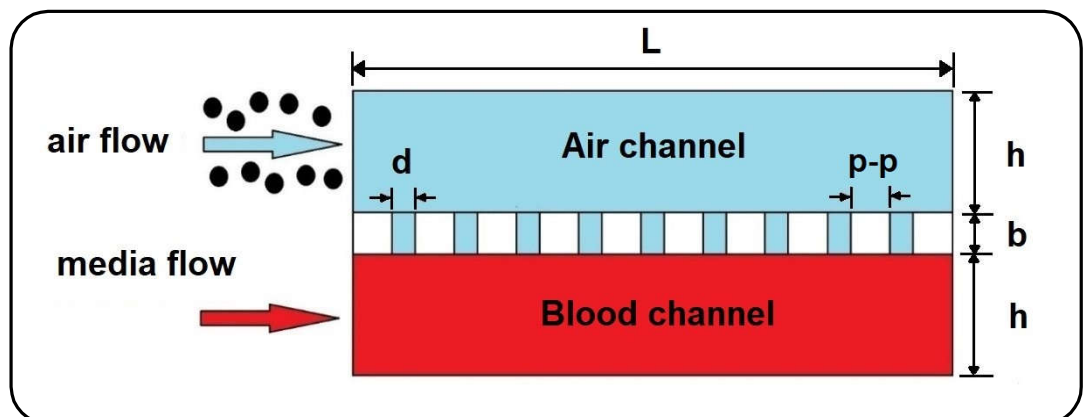

**Figure 2.** 2D model of airborne delivery of NPs into a gas-liquid dual-channel microdevice with a thin, porous membrane.

The Lagrangian approach is used to model the dynamics of NPs under the action of gravity and hydrodynamic forces arising from the motion of the fluid:

$$m_p \frac{du_p^i}{dt} = F_d^i + F_b^i + m_p \left(1 - \frac{\rho_i}{\rho_p}\right) g, \quad (4)$$

where  $m_p$  and  $\rho_p$  are the particle mass and density, and  $u_p^i$  indicates the particle velocity in air and media channels, respectively. The right-hand side of Eq. (4) is the summation of drag force ( $F_d^i$ ), the Brownian force ( $F_b^i$ ), and the particle's buoyant weight, while the gravity acceleration is considered to be perpendicular to the flow direction. The drag force in Eq. (4) is determined in accordance with Stokes law as follows [27]:

$$F_d^i = 3\pi\mu_i(u_i - u_p^i)d_p, \quad (5)$$

Also, Brownian force exerted on particles at each time step taken by the numerical solver could be attained as [28]:

$$F_b^i = \zeta_i \sqrt{6\pi k_B \mu_i T_i d_p / \Delta t}, \quad (6)$$

where  $T_i$  is the fluid temperature, which is considered to be at a constant level of 37°C, and  $\Delta t$  represents the time step.  $\zeta_i$ , which indicates the direction of Brownian force, refers to a vector whose components are randomly selected with a Gaussian distribution [28]. Inertial lift force contribution is neglected in Eq. (4) since the particle Reynolds number is significantly smaller than 1 ( $Re_p = \rho_i u_i d_p^2 / \mu_i l$ ), resulting in viscous forces dominance [29].

Fluid flow boundary conditions in the air and media channels are considered as constant inlet velocity, zero outlet pressure, and no-slip on all solid-fluid interfaces. Furthermore, the top surface of the membrane is employed as the sticky boundary condition for the injected airborne NPs allowing evaluation of particle deposition in the air channel. On the other hand, the pass-through boundary condition is applied to the air-media interfaces to allow NPs to enter the media channel unimpededly. It is worthwhile to note that the numerical simulation is terminated once all the transferred particles flow out of the media channel.

### 3. Model Verification

In this section, comparative studies against accessible data as well as an experimental study are conducted to establish the accuracy of the present numerical study. Accordingly, four limiting-case verifications are considered by setting the membrane's porosity equal to zero.

#### 3.1. Verification of numerical results with analytical data

In the absence of solid particles, the first verification study compares the dimensionless axial fluid velocity in the middle of the air channel with analytical data for a 2D steady laminar flow between two fixed parallel plates in Ref. [30]. For this purpose, fluid velocity and vertical distance from the substrate are normalized with respect to the inlet velocity of 0.3 mm/s and the channel height of 100  $\mu\text{m}$ . As depicted in Figure 3a, a fair agreement is observed between the results of the current study and those of Ref. [30].

#### 3.2. Verification of numerical results with other numerical studies

##### 3.2.1. Verification with a 2D model


Next, the normalized mean concentration of particles with a diameter of 1  $\mu\text{m}$  along the air channel is compared with that obtained by Saidi et al. [21], who developed a customized numerical code to track 2D dynamics of particles under Drag and Brownian forces between two parallel plates. Accordingly, a fully developed inlet flow regime with a mean velocity ( $\bar{u}$ ) of 0.05 m/s and channel height ( $h$ ) of 1 mm is considered. The concentration of particles is calculated by partitioning the computational space into equal bandwidths along the channel length and then dividing the number of particles in each band to the volume of each bandwidth. Finally, distance from the entrance and particle concentration are nondimensionalized respectively with respect to a specific length of  $3hPe/16$ ,



and initial concentration ( $C_0 = 10^5/\text{m}^2$ ) [21].  $Pe = 2\bar{u}h/D$  stands for the Peclet number, where  $D (= 2.96 \times 10^{-11}\text{m}^2/\text{s})$  is diffusion coefficient. The outcome, as shown in Figure 3b, demonstrates a good agreement with Ref. [21].

### 3.2.2. Verification with a 3D model

Subsequently, the correctness of the developed finite element model is examined to evaluate the deposition of airborne NPs. With the definition of "the ratio between the number of deposited particles on the substrate and the number of total released particles" for the deposition rate, the third verification study compares the deposition rate obtained through the current 2D model with that reported for a 3D model developed by Arefi et al. [22]. All adjustments for boundary conditions are taken into account according to Ref. [22]. Here, the effect of channel depth is also surveyed, enabling the "Shallow Channel" interface in the 2D model. Figure 3c compares the results obtained for a 2D channel with finite and infinite depth and the 3D model of Ref. [22], where the independency of deposition rate to the channel depth as well as an excellent agreement between these three is perceivable.

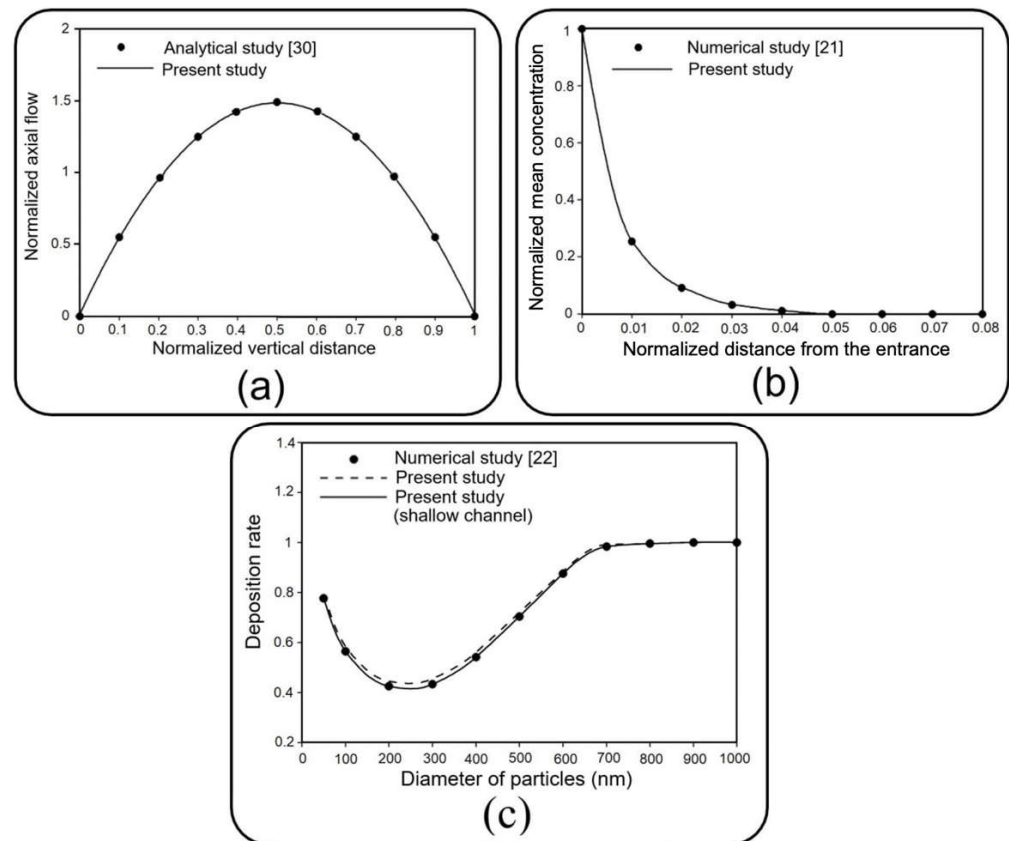


**Figure 3.** Comparison of the present numerical results with (a) analytical data in Ref. [30] for a 2D airflow between two parallel plates. Axial fluid velocity and vertical distance from the substrate are normalized with respect to the inlet velocity of 0.3 mm/s and the channel height of 100  $\mu\text{m}$ ., (b) numerical data in Ref. [21] for the mean concentration of particles with a diameter of 1  $\mu\text{m}$  along two parallel plates. Distance from the entrance and particle concentration are nondimensionalized respectively with respect to a specific length of  $3hPe/16$ , and initial concentration ( $C_0 = 10^5/\text{m}^2$ ).  $Pe = 2\bar{u}h/D$  is the Peclet number, where  $D (= 2.96 \times 10^{-11}\text{m}^2/\text{s})$  is diffusion coefficient., and (c) numerical result of Ref [22] for deposition rate of NPs with various diameters on the substrate of an air channel.


### 3.3. Qualitative verification of the numerical results with experimental data

Besides verification against the analytical and numerical data in the literature, an experimental study was accomplished to support the results of the present numerical model. The experiment was carried out with the injection of particles into a microchannel under

a water flow. Therefore, a numerical simulation was developed in accordance with the experimental parametric values to compare the obtained results from the two studies. Accordingly, a polydimethylsiloxane (PDMS) microchannel with rectangular cross-section was fabricated using a silicone mold (see Figure 4a). The mold was made with maskless ultraviolet (UV) lithography method, as shown in Figure 4b. A silicon wafer coated with a positive photoresist was exposed to direct UV laser to transfer the channel design on it. Subsequently, the wafer was dry etched to engrave the microchannel mold. Then, a 10:1 mixture of PDMS was casted on the mold and the microchannel was sealed with a glass slide to finalize the fabrication procedure (see Figure 4b). A syringe pump was used to inject the particles into the channel under different fluid velocities (see Figure 5 for the experimental setup). In order to have a similar inlet boundary condition to that of the numerical model, the particles were first accumulated at the entrance of the inlet and injected altogether into the channel. Fluid injection was stopped once the particles reached the channel outlet or deposited entirely.

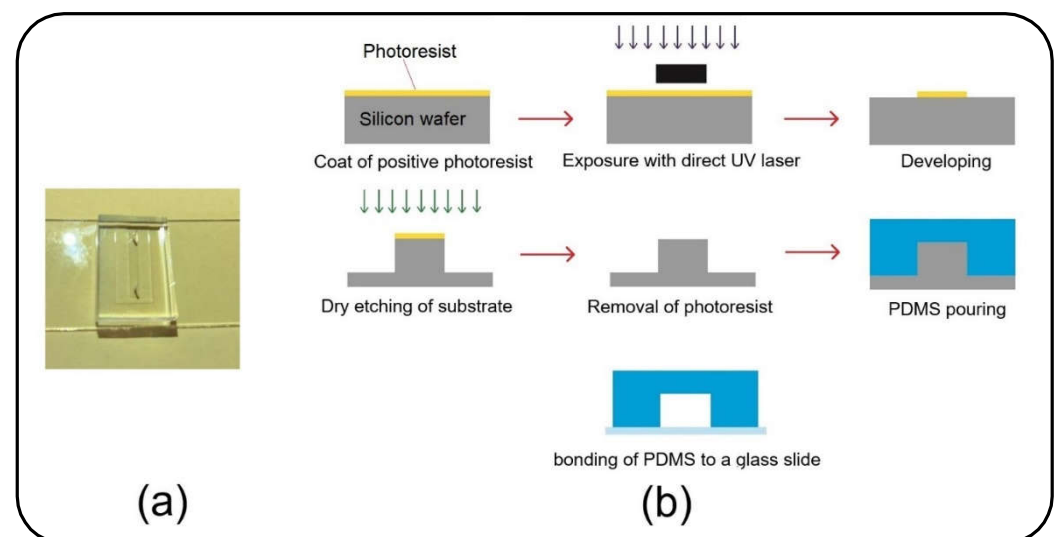

**Figure 4.** (a) Microfluidic device, which is bonded to a glass slide and contains a channel with one inlet and one outlet; (b) Schematic diagram of the fabrication process of the microfluidic device.

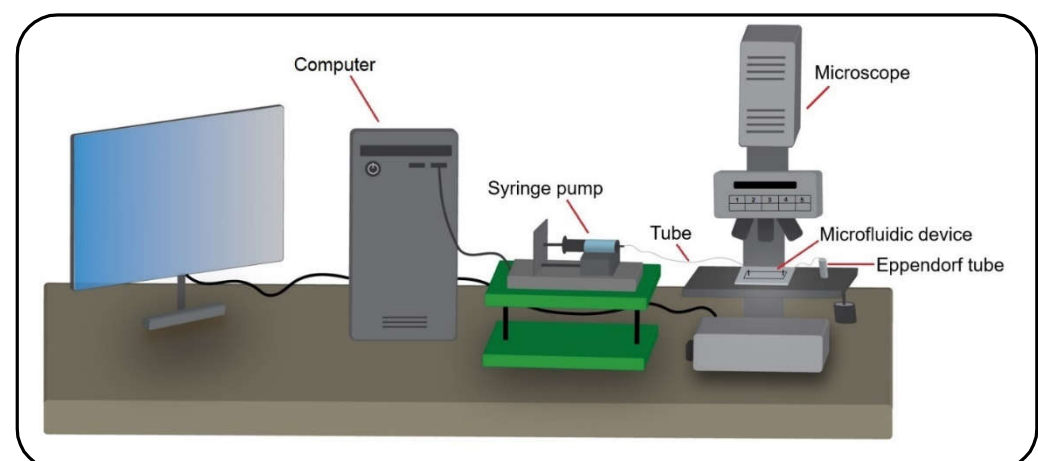

**Figure 5.** Schematic diagram of the experimental setup for injecting the particles into a microfluidic device using a syringe pump and monitoring their dynamics throughout the device with a microscope.

Magnetic particles of diameter  $1\ \mu\text{m}$  and  $10\ \mu\text{m}$  were used in the experiments to investigate their sedimentation on the channel substrate under three different water flow velocities. In addition to more deposition efficiency due to their higher inertia and

dominant buoyant weight, better control on injection and easier tracing are other main reasons for selecting these particles. The experimental parameter values, including the physical properties of particles, fluid velocities, and the dimension of the microchannel, are listed in Table.1.

**Table 1.** The values of the parameter used for the experimental test.


Diameter of Particles ( $d_p$ ) [ $\mu\text{m}$ ]	Density of Particles ( $\rho_p$ ) [ $\text{kg/m}^3$ ]	Dimension of Channel ( $w \times h \times l$ ) [ $\mu\text{m}^3$ ]	Fluid velocity ( $u_{m,0}$ ) [mm/s]	Flow rate [ $\mu\text{L/min}$ ]
1	2200	2000×100×15000	0.03 and 0.1	0.36 and 1.2
10	1470	2000×300×15000	0.1 and 0.3	3.6 and 10.8

Figure 6 qualitatively compares the trend of particle deposition obtained from the numerical and experimental studies under four different cases. The experimental results are actual images showing the particle deposition rate on the bottom layer of the microchannels. These images were obtained from two different parts of the channel substrate, one from the first half of the channel and the other from its second half.

First, the particles with a diameter of 1  $\mu\text{m}$  were injected into the channel with a height of 100  $\mu\text{m}$  under a fluid velocity of 0.3 mm/s. Due to the dominance of drag force over the buoyant weight, all the particles were washed out from the channel without any deposition on the substrate (data not shown). Then, the dynamics of particles were examined with a lower fluid velocity of 0.1 mm/s and 0.03 mm/s. Under the fluid velocity of 0.1 mm/s, the particles again streamed fast toward the microchannel outlet, resulting in a low deposition rate along the channel length (see Figure 6a). The fluid velocity, therefore, was reduced to 0.03 mm/s so that the particles could uniformly distribute all over the channel substrate and demonstrated a higher deposition rate, Figure 6b.

There is a mild deposition gradient along the channel width due to the parabolic profile of the fluid velocity in the channel. Moreover, on the substrate next to the channel side walls, the deposition rate is very low as a consequence of the no-slip boundary condition. In the second part of the experiment, particles with a diameter of 10  $\mu\text{m}$  were examined under fluid velocities of 0.1 mm/s and 0.3 mm/s (see Figure 6c and 6d). The height of the microchannel was increased to 300  $\mu\text{m}$  to allow the particles to easily move inside the channel. The distribution of particles on the substrate of the channel reveals that particles with a diameter of 10  $\mu\text{m}$  under the fluid velocity of 0.1 mm/s provide a concentrated deposition at the channel's entrance. However, an increase in the fluid velocity to 0.3 mm/s drives the particles fast forward, resulting in a uniform particles' distribution on the channel substrate. The experimental results for deposition and distribution of the particles on the substrate of the microchannel show a good agreement with the numerical results.



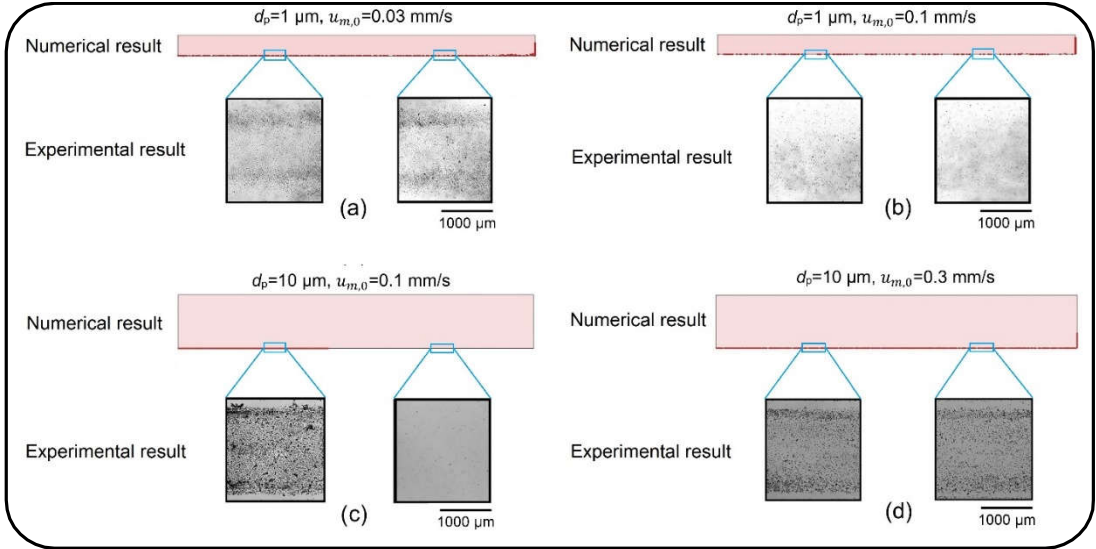

**Figure 6.** Qualitative comparison of distribution and deposition of the particles on the microchannel substrate obtained from numerical and experimental studies. (a)  $d_p = 1 \mu\text{m}$ ,  $u_{m,0} = 0.03 \text{ mm/s}$ , (b)  $d_p = 1 \mu\text{m}$ ,  $u_{m,0} = 0.1 \text{ mm/s}$ , (c)  $d_p = 10 \mu\text{m}$ ,  $u_{m,0} = 0.1 \text{ mm/s}$ , and (d)  $d_p = 10 \mu\text{m}$ ,  $u_{m,0} = 0.3 \text{ mm/s}$ .

4. Numerical Results


The current numerical parametric study investigates the dynamics of airborne NPs in a gas-liquid dual-channel lung-on-a-chip device with a thin, porous membrane using Eqs. (2-4). Accordingly, the impact of fluid flow velocity, membrane porosity, and particle diameter, as dominant factors, are analyzed on the dispersion of the particles in both air and media channels as well as their deposition and translocation. Numerical results are confined only to some specific cases due to the computational limitations as well as for the sake of brevity. The diameter of solid particles is assumed to be ranging between 10 to 900 nm, according to their high deposition rate reported in the alveolar region [4]. The effect of membrane porosity is examined for pore diameters ( $d$ ) of 3 and 10 μm, and pore to pore distances ( $p - p$ ) of 5 and 10 μm. The other numerical values used for simulations are all listed in Table 2.

**Table 2.** The values of the parameter used for the numerical simulations.

Parameters	Values	Descriptions	Reference
$h$	100 μm	Height of the channels	[31]
$l$	2 mm	Length of the channels	[22]
$d$	10 μm, 3 μm	Diameter of the membrane pore	[31,32]
$b$	10 μm	Thickness of the membrane	[8]
$\rho_p$	1180 kg/m <sup>3</sup>	Density of particles	[22]
$\rho_m$	1000 kg/m <sup>3</sup>	Density of media	[33]
$\mu_m$	0.718 mPa.s	Viscosity of media	[33]
$\rho_a$	1.123 kg/m <sup>3</sup>	Density of air	[34]
$\mu_a$	0.019 mPa.s	Viscosity of air	[34]
$u_{m,0}$	0.3 mm/s, 1mm/s	Media velocity at inlet	[23,31]
$u_{a,0}$	0.3 mm/s, 1mm/s	Air velocity at inlet	[22]

Before presenting the main results, a brief discussion is presented here to investigate the dynamics of NPs injected with an aqueous solution, which substitutes aerosol injection in many relevant experimental studies [8,11,12]. Accordingly, the pore diameter of 10 μm and pore-to-pore distance of 10 μm are taken into consideration, and the deposition rate and transfer rate are compared in Figure 7 for NPs injected via air and media flow into

the upper channel of the device. As previously mentioned, the deposition rate is referred to as the proportion of the total released particles that deposit on the channel substrate. Similarly, the transfer rate defines the ratio between the number of transferred particles to the media channel and the number of released particles. Obtained results demonstrate a noticeable decrease in deposition/transfer rate when media flow is used for the injection of NPs, regardless of their size. To put it clearly, particles follow the fully-developed parabolic profile of media velocity with a lower chance of settling on the substrate or passing through it (data not shown for brevity). Buoyant weight almost fades for submerged particles with a density of the same order as the fluid, which explains the reduction in deposition/transfer rate, especially for large particles. Furthermore, by increasing the fluid viscosity, the drag force dominates the Brownian force, which plays a key role in the deposition of small NPs. Thus, one can draw the conclusion that injecting through an aqueous solution leads to less efficient particle deposition/translocation, and accordingly, air flow injection should be taken into consideration.

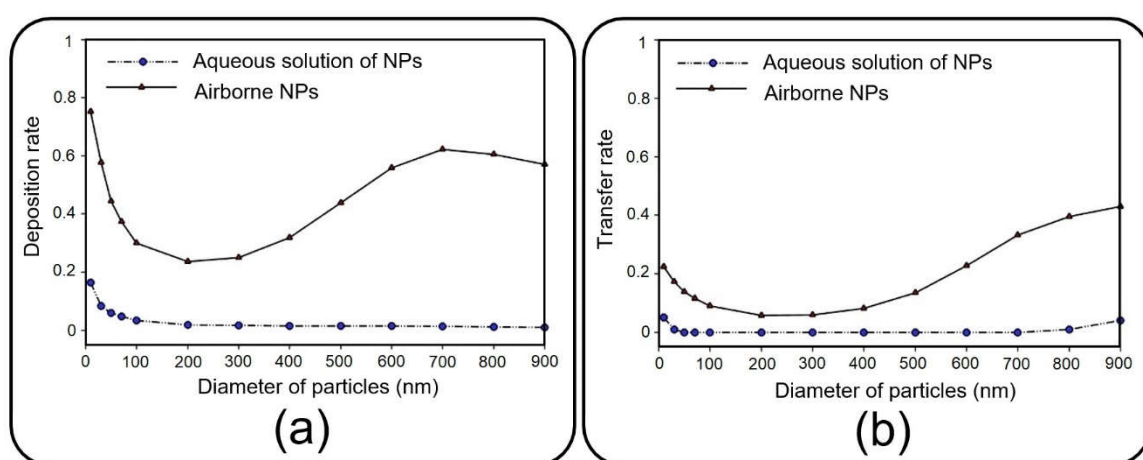


**Figure 7.** (a) Deposition rate and (b) transfer rate of the media- and air-induced NPs in the top channel of the lung-on-a-chip device when the fluid velocity is 0.3 mm/s, and both pore diameter and pore-to-pore distance are 10  $\mu$ m.


#### 4.1. Deposition of nanoparticles

This section deals with the sedimentation of airborne NPs in the air channel of the lung-on-a-chip device with a focus on the deposition rate and distribution efficiency. Figure 8 depicts the deposition rate against particle diameter for different membrane porosities and air inflow velocities of 0.3 and 1 mm/s. The results show that the deposition rate declines by increasing the particle diameter up to 200 nm regardless of the inlet velocity. The reason behind this decay is related to the dominance of Brownian diffusion, which is the main particle deposition mechanism for particles of diameter less than 100 nm according to Stokes–Einstein expression [27,35,36]. On the other hand, as could be deduced from Eqs. (4-6), gravity acceleration becomes more dominant by increasing the particle diameter, while the Brownian effect diminishes. This consequently results in higher deposition rates as the particles enlarge, which can be observed in Figure 8 for diameters larger than 200 nm. A comparison between Figures 8a and 8b implies an overall decrease in deposition rate by intensifying the inlet flow rate, which makes a larger fraction of NPs leave the device through the air channel outlet. However, both cases follow a similar trend except for particles larger than 700 nm, demonstrating a downtrend of deposition rate for inflow velocity of 0.3 mm/s. By comparing the results of Figure 8a and those of Figure 12a, it is observed that more than 95% of these injected big particles tend to either sediment on the air channel substrate or pass through the perforated membrane with a growing transfer rate against the particle size. Therefore, one can conclude that this unexpected behavior is not linked with blowing NPs off the device but rather with a higher transfer rate into the media channel. Indeed, lower inflow velocity magnitude results in slower axial fluid

velocity in the boundary layer above the porous area and prolonged regional residence time, which consequently provide more probability for heavier particles to pass through the membrane. The idea is explicitly illustrated through a series of snapshots in Figure 9, where the trajectory of an initially inert 900 nm particle is compared in the porous region for inflow velocities of 0.3 and 1 mm/s. Such behavior also leads to more dependency of larger NPs' deposition on membrane porosity, which is supported by the divergence of deposition rate curves corresponding with different porosities in Figure 8.

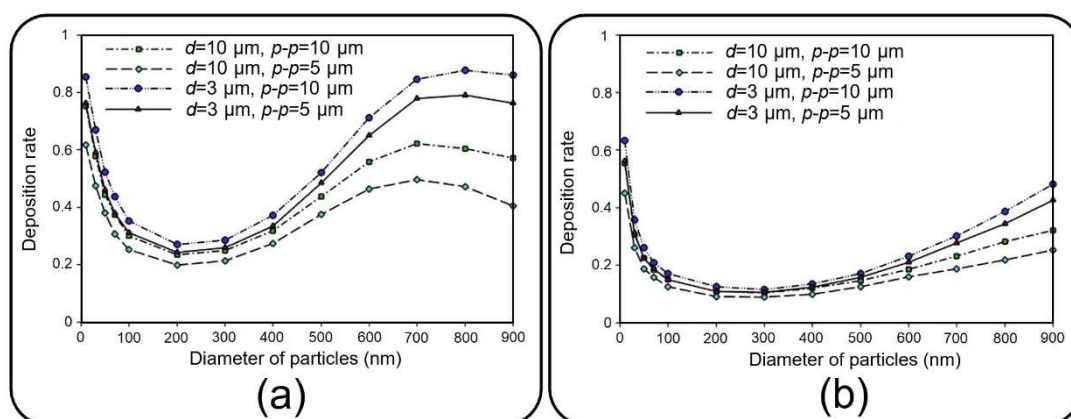

**Figure 8.** Deposition rate of airborne NPs of diameter ranging from 10 nm to 900 nm on the substrate of the air channel with different membrane porosities and airflow velocities of (a) 0.3 mm/s and (b) 1 mm/s.

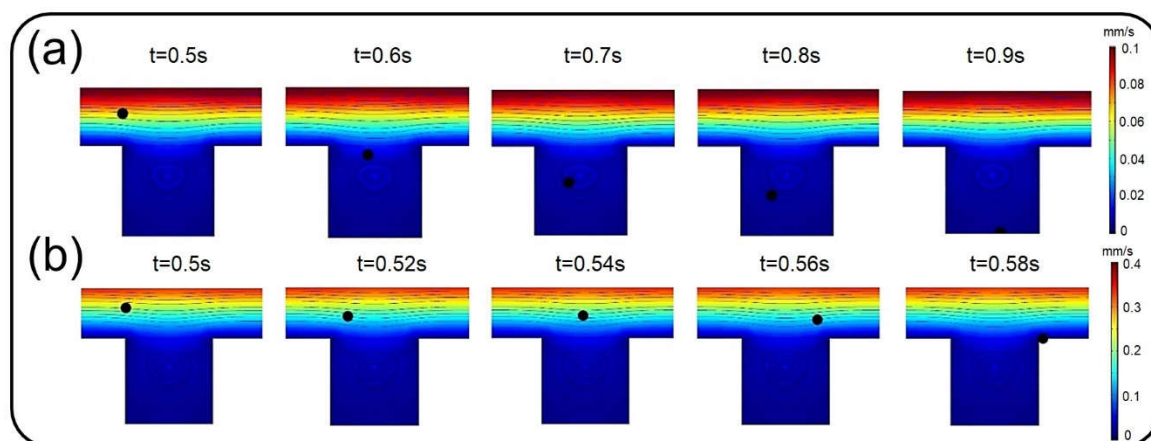


**Figure 9.** Trajectory of an initially inert 900 nm particle in the porous region for inflow velocities of (a) 0.3 mm/s and (b) 1 mm/s.


Beside the high deposition rate of the injected solid NPs, their better distribution on the channel substrate is another significant factor in toxicological and pharmaceutical studies to attain an effective biochemical impact on cultured cells. Here, the distribution of NPs is mathematically described in terms of the mean value and standard deviation of their position [37].

Figure 10 depicts dimensionless distribution indexes of deposited NPs on the air channel substrate under two air inflow velocities, which are normalized with respect to channel length here. Since membrane porosity has no remarkable effect on **statistical** characteristics of particle distribution due to the regular alignment of pores, only a single case with a pore diameter of 10  $\mu\text{m}$  and pore-to-pore distance of 10  $\mu\text{m}$  is considered. Distribution efficiency can simply be assessed against an ideal uniform deposition with normalized mean value of 0.5 and a standard deviation of  $1/\sqrt{12}$  (shown with a solid red line in Figure. 10) [37].

Under an airflow velocity of 0.3 mm/s, both small and large particles demonstrate low values of the mean location and standard deviation, indicating a concentrated deposition at the entrance of the channel. Increasing the airflow velocity would not alter the results unless for particles larger than 600 nm or smaller than 50 nm, giving rise to a significantly widened distribution range. Although the uniform distribution achieved by higher inflow velocity seems to be desirable, it should be noted that the deposition rate would be unfavorably affected in this case. Therefore, depending on the application, a tradeoff between deposition rate and distribution uniformity should be considered to obtain proper particle size and inflow velocity values. To provide a better insight into the problem, snapshots from the distribution of 900 nm particles are provided in Figure 11.

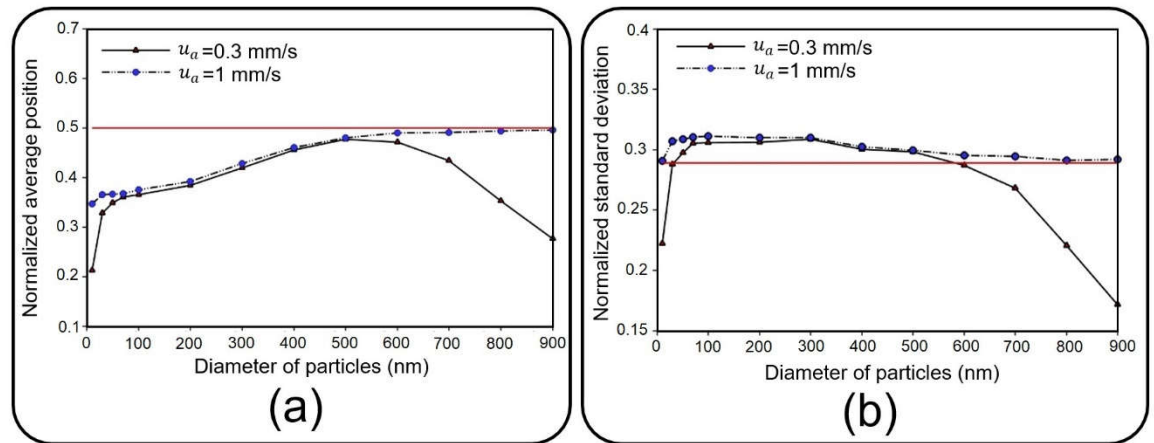

**Figure 10.** Normalized (a) average position and (b) standard deviation of deposited NPs of diameter ranging from 10 nm to 900 nm on the substrate of the air channel with pore diameter and pore to pore distance of 10  $\mu$ m under two different fluid velocities of 0.3 mm/s and 1 mm/s. The solid red line corresponds with an ideal deposition.

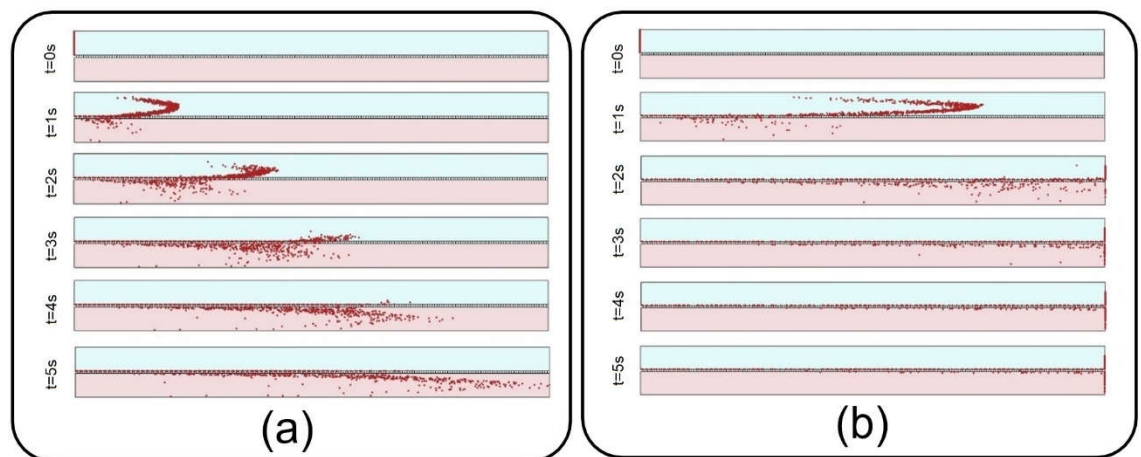


**Figure 11.** Snapshots from transient distribution of NPs with a diameter of 900 nm in the lung-on-a-chip device with pore diameter and pore-to-pore distance of 10  $\mu$ m under the fluid velocity of (a) 0.3 mm/s, and (b) 1 mm/s.

#### 4.2. Translocation of nanoparticles

This section deals with the translocation of airborne NPs into the media channel of the lung-on-a-chip device, mainly analyzing transfer rate and distribution efficiency. Figure 12 compares the transfer rate of NPs for different membrane porosities and inflow velocities. A higher translocation efficiency seems achievable by increasing the former and


decreasing the latter. The obtained results show that for constant membrane porosity and inlet velocity, the transfer rate declines by increasing the particle diameter up to 200 nm, whereafter it starts to go up. Higher transfer rates arise from Brownian diffusivity for small particles and dominance of gravity force, as well as longer residence time in the porous regions for large particles.

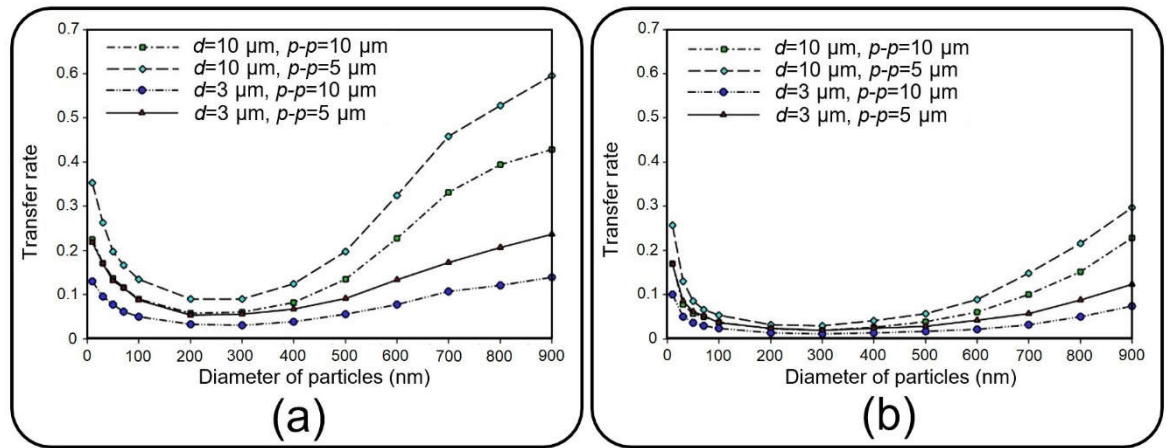


**Figure 12.** Transfer rate of NPs of diameter ranging from 10 nm to 900 to the media channel of the lung-on-a-chip device with different membrane porosities considering equal inflow velocities of (a) 0.3 mm/s and (b) 1 mm/s for air and media channels.

Distribution of NPs inside the media channel is also of great importance especially for targeted particle delivery applications. Since submerged particles with a density close to that of fluid would follow the media velocity profile regardless of inflow velocity, the results are presented only for the inlet velocity of 0.3 mm/s. Accordingly, vertical distribution of transferred NPs are assessed at the outlet of media channel utilizing Eqs. (4-5) with  $N$  representing the number of transferred particles and  $x_n$  showing the vertical position of each particle. Here, the average position and standard deviation are normalized with respect to media channel height, and similar to the previous section, are then assessed against an ideal uniform distribution (shown with the solid red line in Figure 13). Higher average position and smaller standard deviation for large particles in Figure 13 indicate their tendency to accumulate close to the media channel's top surface, where the endothelial cells are normally cultured. On the other hand, smaller particles demonstrate a higher penetration power, which is due to their higher vertical velocity magnitude while crossing the membrane as well as relatively strong Brownian force in the medium. Moreover, a more uniform distribution is observed for medium-sized particles with a diameter range of 100-300 nm. For a better vision of the impact of size, one can compare the snapshots from the distribution of 10 nm particles in Figure 14 with those obtained from 900 nm particles in Figure 11a.



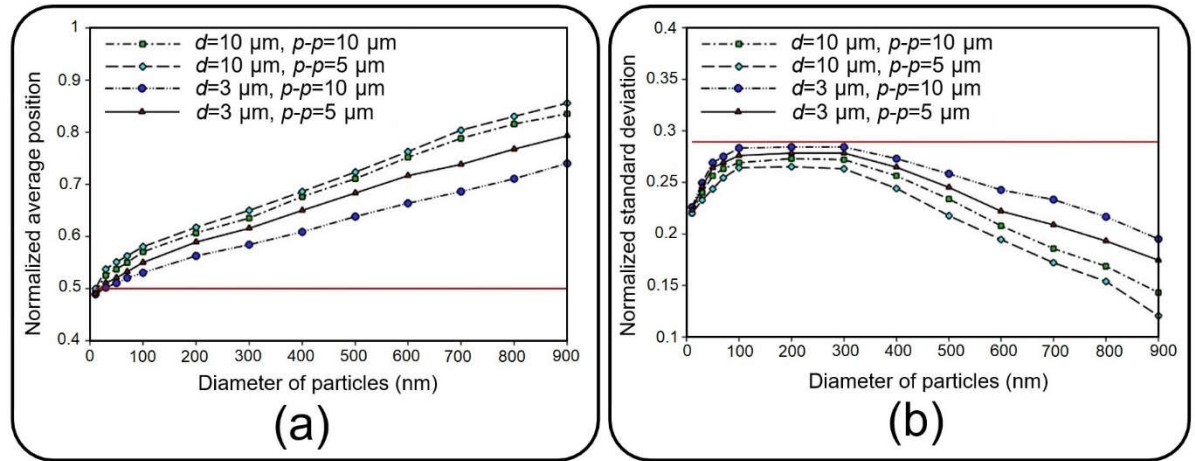


**Figure 13.** Normalized (a) average position and (b) standard deviation of transferred NPs of diameter ranging from 10 nm to 900 at the outlet of the media channel in the lung-on-a-chip device with different membrane porosities under the fluid velocity of 0.3 mm/s. The solid red line corresponds with an ideal distribution in the media channel.

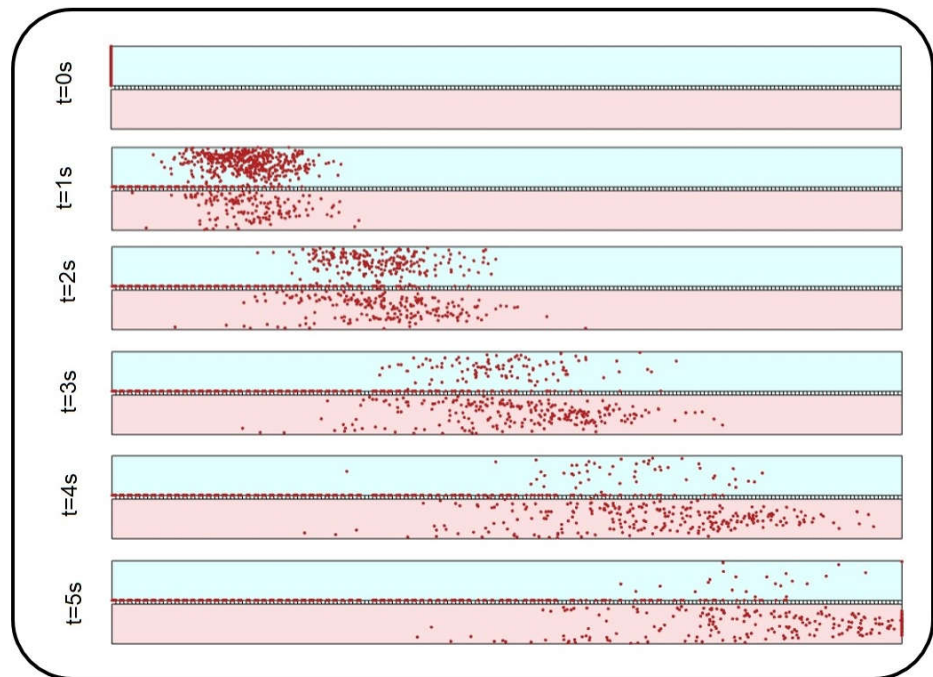

**Figure 14.** Snapshots from transient distribution of particles with a diameter of 10 nm in the lung-on-a-chip device with pore diameter and pore-to-pore distance of 10  $\mu\text{m}$  and fluid velocity of 0.3 mm/s.

In addition to distribution efficiency, the current study investigates the transient evolution of transferred NPs as a significant factor in toxico-pharmacokinetic analyses [38]. First, the relative concentration, which is defined by the ratio of total injected particles that flow out through the outlet of the media channel, is recorded, and then, a numerical differentiation is utilized to obtain the time derivative of the data. After a Gaussian curve fitting, final results are depicted in Figure 15 for different membrane porosities and inlet velocities. Figure 15, which is known as the so-called concentration-time plot [38], provides important details describing the behavior of transferred NPs to the media channel, such as area under each curve, which is equal to the transfer rate (see Figure 12), maximum relative concentration rate ( $c_{max}$ ), and time to reach this maximal value ( $t_{max}$ ). For example, it is shown that 10 nm particles demonstrate the highest  $c_{max}$ , which is significantly augmented by increasing the inflow velocity. Moreover, it is evident that smaller particles

display a faster transmission with a lower  $t_{max}$ . Although the overall value of  $c_{max}$  grows by increasing the membrane porosity and inflow velocity, it should be noted that this may also considerably change  $t_{max}$  depending on the particle size.

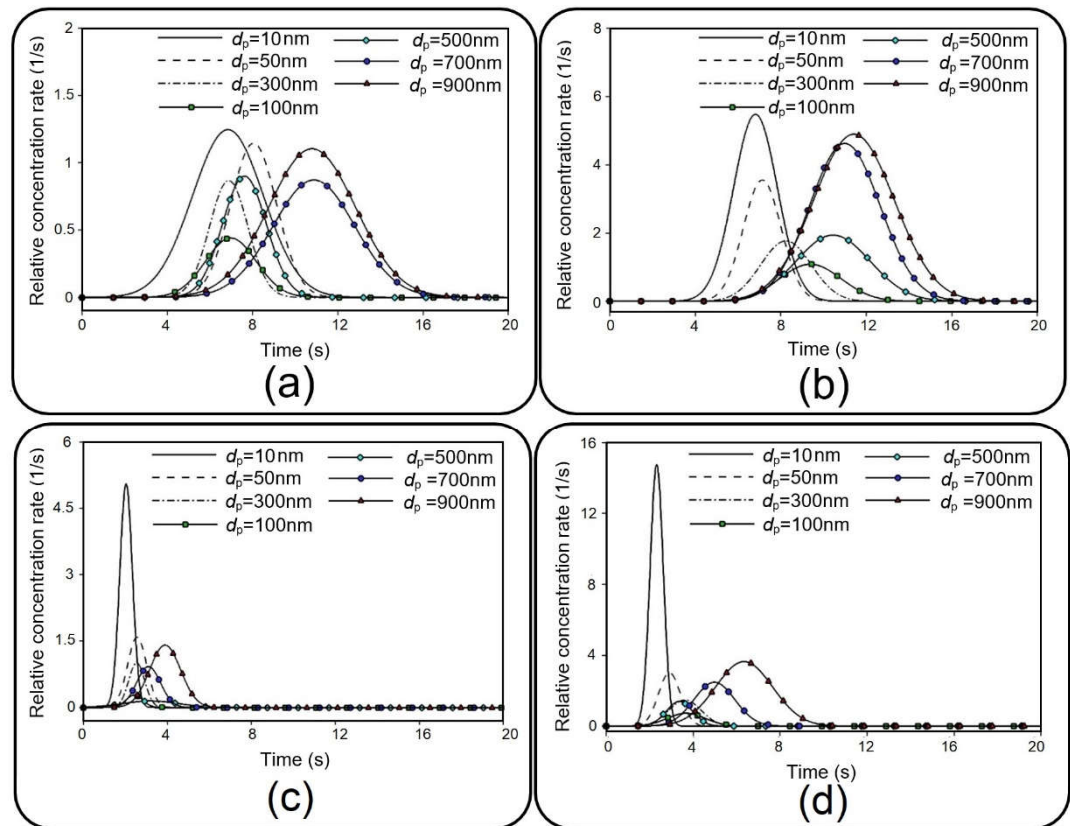

**Figure 15.** Transient relative concentration rate for NPs with different diameters. (a)  $d = 3 \mu\text{m}$ ,  $p = 10 \mu\text{m}$ ,  $u_a = 0.3 \text{ mm/s}$ , (b)  $d = 10 \mu\text{m}$ ,  $p = 5 \mu\text{m}$ ,  $u_a = 0.3 \text{ mm/s}$ , (c)  $d = 3 \mu\text{m}$ ,  $p = 10 \mu\text{m}$ ,  $u_a = 1 \text{ mm/s}$ , and (d)  $d = 10 \mu\text{m}$ ,  $p = 5 \mu\text{m}$ ,  $u_a = 1 \text{ mm/s}$ .

## 5. Conclusion

With a promising potential in recapitulating *in vivo* conditions, lung-on-a-chip technology has recently attained the attention of the research society. This dual-channel device with a sandwiched porous membrane enables particle tracing in air and media phases simultaneously, which is an essential prerequisite for further toxicological and pharmaceutical studies. Despite this remarkable capability, a detailed investigation into the dynamics of NPs in this device has been overlooked in the literature. Here, a comprehensive numerical parametric study was conducted to study the role of various hydrodynamical and geometrical properties on the dynamics of airborne NPs. Accordingly, the impact of fluid flow velocity, membrane porosity, and particle diameter were examined on the dispersion of the particles in both air and media channels, as well as their deposition and translocation. Consistent with the experimental observation reported in the literature, we numerically showed that the aerosol injection of NPs provided far more efficient deposition/translocation than the aqueous solution. Although very small particles ( $d_p < 50 \text{ nm}$ ) as well as very large ones ( $d_p > 700 \text{ nm}$ ) demonstrated a high deposition rate, they tended to sediment close to the entrance of the channel for low inflow velocities, which could be undesirable for many applications demanding a uniform distribution. On the other hand, a higher inflow velocity provided a more uniform distribution; however, it also resulted in lower deposition and translocation rates. Therefore, it can be concluded that medium-sized particles ( $500 \text{ nm} < d_p < 700 \text{ nm}$ ) are more appropriate for uniform distribution with lower inflow velocities. It was demonstrated that the translocation of NPs into the

media channel became more efficient by reducing the particle size due to Brownian diffusivity and also by increasing the particle residence time in the porous region as a consequence of gravity force dominance for large particles. However, smaller particles showed a better distribution in the media channel than larger ones. Therefore, the results of this paper propose optimizing particle size as well as inflow velocity and membrane porosity depending on the objectives of biomedical investigations. Even though the current numerical analysis is carried out with some simplifications, such as neglecting the cultured cell layers, it takes the first step towards a perceptive insight into the dynamics of the NPs in the lung-on-a-chip device. As a reliable complementary method to reducing experimental cost, time and efforts, this study can be beneficial for future preclinical studies on pulmonary pathology associated with inhaled hazardous and toxic environmental particles, as well as therapeutic studies for developing inhalation drug delivery.

**Author Contributions:** Conceptualization, Z.S., P.A. and N.K.; methodology, Z.S.; software, Z.S.; validation, Z.S.; investigation and resources, Z.S.; writing—original draft preparation, Z.S.; writing—review and editing, P.A., N.K. and C.G.; visualization, Z.S.; supervision, P.A., N.K. and C.G.; funding acquisition, Z.S., P.A. All authors have read and agreed to the published version of the manuscript.

**Funding:** This research received no external funding.

**Institutional Review Board Statement:** Not applicable

**Informed Consent Statement:** Not applicable

**Data Availability Statement:** The data (movies and images) that support the findings of this study are available from the corresponding author upon reasonable request.

**Acknowledgments:** Z.S. and P.A. would like to acknowledge the Shahrood University of Technology, which supported this study and École polytechnique fédérale de Lausanne for supporting the experimental part of this study and its specific infrastructure for computational resources. Z.S. and P.A. also want to thank Swiss Government Excellence Scholarship. N.K. acknowledges funding support from the Australian Research Council (ARC) Discovery Early Career Research Award (DECRA) DE220100205.

**Conflicts of Interest:** The authors declare no conflict of interest.

## References

- Knudsen, L.; Ochs, M. The Micromechanics of Lung Alveoli: Structure and Function of Surfactant and Tissue Components. *Histochem. Cell Biol.* **2018**, *150*, 661–676. DOI: 10.1007/s00418-018-1747-9.
- Li, J.J.; Muralikrishnan, S.; Ng, C.-T.; Yung, L.-Y.L.; Bay, B.-H. Nanoparticle-Induced Pulmonary Toxicity. *Exp. Biol. Med.* **2010**, *235*, 1025–1033. DOI: 10.1258/ebm.2010.010021.
- Nel, A.; Xia, T.; Mädler, L.; Li, N. Toxic Potential of Materials at the Nanolevel. *Science*. **2006**, *311*, 622–627. DOI: 10.1126/science.1114397.
- Amararathna, M.; Goralski, K.; Hoskin, D.W.; Rupasinghe, H.P.V. Pulmonary Nano-Drug Delivery Systems for Lung Cancer: Current Knowledge and Prospects. *J. Lung Heal. Dis.* **2019**, *3*. DOI: 10.29245/2689-999X/2019/2.1148.
- Madl, A.K.; Plummer, L.E.; Carosino, C.; Pinkerton, K.E. Nanoparticles, Lung Injury, and the Role of Oxidant Stress. *Annu. Rev. Physiol.* **2014**, *76*, 447–465. DOI: 10.1146/annurev-physiol-030212-183735.
- Xia, T.; Li, N.; Nel, A.E. Potential Health Impact of Nanoparticles. *Annu. Rev. Public Health* **2009**, *30*, 137–150. DOI: 10.1146/annurev.publhealth.031308.100155.
- Raftis, J.B.; Miller, M.R. Nanoparticle Translocation and Multi-Organ Toxicity: A Particularly Small Problem. *Nano Today* **2019**, *26*, 8–12. DOI: 10.1016/j.nantod.2019.03.010.
- Huh, D.; Matthews, B.D.; Mammoto, A.; Montoya-Zavala, M.; Hsin, H.Y.; Ingber, D.E. Reconstituting Organ-Level Lung Functions on a Chip. *Science*. **2010**, *328*, 1662–1668. DOI: 10.1126/science.1188302.
- Huh, D.; Leslie, D.C.; Matthews, B.D.; Fraser, J.P.; Jurek, S.; Hamilton, G.A.; Thorne, K.S.; McAlexander, M.A.; Ingber, D.E. A Human Disease Model of Drug Toxicity-Induced Pulmonary Edema in a Lung-on-a-Chip Microdevice. *Sci. Transl. Med.* **2012**, *4*, 1–10. DOI: 10.1126/scitranslmed.3004249.
- Jain, A.; Barrile, R.; van der Meer, A.D.; Mammoto, A.; Mammoto, T.; De Ceunynck, K.; Aisiku, O.; Otieno, M.A.; Loudon, C.S.; Hamilton, G.A. Primary Human Lung Alveolus-on-a-chip Model of Intravascular Thrombosis for Assessment of Therapeutics. *Clin. Pharmacol. Ther.* **2018**, *103*, 332–340. DOI: 10.1002/cpt.742.

11. Sedláková, V.; Kloučková, M.; Garlíková, Z.; Vašíčková, K.; Jaroš, J.; Kandra, M.; Kotasová, H.; Hampl, A. Options for Modeling the Respiratory System: Inserts, Scaffolds and Microfluidic Chips. *Drug Discov. Today* **2019**, *24*, 971–982. DOI: 10.1016/j.drudis.2019.03.006.
12. Zhang, M.; Xu, C.; Jiang, L.; Qin, J. A 3D Human Lung-on-a-Chip Model for Nanotoxicity Testing. *Toxicol. Res.* **2018**, *7*, 1048–1060. DOI: 10.1039/C8TX00156A.
13. Moghadas, H.; Saidi, M.S.; Kashaninejad, N.; Nguyen, N.T. A High-Performance Polydimethylsiloxane Electrospun Membrane for Cell Culture in Lab-on-a-Chip. *Biomicrofluidics* **2018**, *12*, 24117. DOI: 10.1063/1.5021002.
14. Quirós-Solano, W.F.; Gaio, N.; Stassen, O.M.J.A.; Arik, Y.B.; Silvestri, C.; Van Engeland, N.C.A.; Van der Meer, A.; Passier, R.; Sahlgren, C.M.; Bouten, C.V.C. Microfabricated Tuneable and Transferable Porous PDMS Membranes for Organs-on-Chips. *Sci. Rep.* **2018**, *8*, 1–11. DOI: 10.1038/s41598-018-31912-6.
15. Ari, A. Jet, Ultrasonic, and Mesh Nebulizers: An Evaluation of Nebulizers for Better Clinical Outcomes. **2014**.
16. Sheidaei, Z.; Akbarzadeh, P.; Kashaninejad, N. Advances in Numerical Approaches for Microfluidic Cell Analysis Platforms. *J. Sci. Adv. Mater. Devices* **2020**. DOI: 10.1016/j.jsamd.2020.07.008.
17. Sheidaei, Z.; Akbarzadeh, P.; Nguyen, N.T.; Kashaninejad, N. A New Insight into a Thermoplastic Microfluidic Device Aimed at Improvement of Oxygenation Process and Avoidance of Shear Stress during Cell Culture. *Biomed. Microdevices* **2022**, *24*, 1–13. DOI: 10.1007/s10544-022-00615-1.
18. Frost, T.S.; Estrada, V.; Jiang, L.; Zohar, Y. Convection–Diffusion Molecular Transport in a Microfluidic Bilayer Device with a Porous Membrane. *Microfluid. Nanofluidics* **2019**, *23*, 1–13. DOI: 10.1007/s10404-019-2283-1.
19. Yacobi, N.R.; Fazlollahi, F.; Kim, Y.H.; Sipos, A.; Borok, Z.; Kim, K.-J.; Crandall, E.D. Nanomaterial Interactions with and Trafficking across the Lung Alveolar Epithelial Barrier: Implications for Health Effects of Air-Pollution Particles. *Air Qual. Atmos. Heal.* **2011**, *4*, 65–78. DOI: 10.1007/s11869-010-0098-z.
20. Mosquera, J.; García, I.; Liz-Marzán, L.M. Cellular Uptake of Nanoparticles versus Small Molecules: A Matter of Size. *Acc. Chem. Res.* **2018**, *51*, 2305–2313. DOI: 10.1021/acs.accounts.8b00292
21. Saidi, M.S.; Rismanian, M.; Monjezi, M.; Zendeabad, M.; Fatehiboroujeni, S. Comparison between Lagrangian and Eulerian Approaches in Predicting Motion of Micron-Sized Particles in Laminar Flows. *Atmos. Environ.* **2014**, *89*, 199–206. DOI:10.1016/j.atmosenv.2014.01.069.
22. Amin Arefi, S.M.; Tony Yang, C.W.; Sin, D.D.; Feng, J.J. Simulation of Nanoparticle Transport and Adsorption in a Microfluidic Lung-on-a-Chip Device. *Biomicrofluidics* **2020**, *14*, 44117. DOI:10.1063/5.0011353.
23. Moghadas, H.; Saidi, M.S.; Kashaninejad, N.; Nguyen, N.-T. Challenge in Particle Delivery to Cells in a Microfluidic Device. *Drug Deliv. Transl. Res.* **2018**, *8*, 830–842. DOI: 10.1007/s13346-017-0467-3.
24. COMSOL Multiphysics 5.6, COMSOL AB, Stockholm, Sweden, [www.comsol.com](http://www.comsol.com).
25. Liu, C.; Zhou, G.; Shyy, W.; Xu, K. Limitation Principle for Computational Fluid Dynamics. *Shock Waves* **2019**, *29*, 1083–1102.
26. Barisam, M.; Saidi, M.S.; Kashaninejad, N.; Vadivelu, R.; Nguyen, N.-T. Numerical Simulation of the Behavior of Toroidal and Spheroidal Multicellular Aggregates in Microfluidic Devices with Microwell and U-Shaped Barrier. *Micromachines* **2017**, *8*, 358. DOI: 10.3390/mi8120358
27. Hinds, W.C. *Aerosol Technology: Properties, Behavior, and Measurement of Airborne Particles*. John Wiley & Sons **1999**. ISBN 0471194107.
28. Zhang, H.; Ahmadi, G. Aerosol Particle Transport and Deposition in Vertical and Horizontal Turbulent Duct Flows. *J. Fluid Mech.* **2000**, *406*, 55–80. DOI: 10.1017/S0022112099007284.
29. Zhang, J.; Yan, S.; Yuan, D.; Alici, G.; Nguyen, N.-T.; Warkiani, M.E.; Li, W. Fundamentals and Applications of Inertial Microfluidics: A Review. *Lab Chip* **2016**, *16*, 10–34. DOI:10.1039/C5LC01159K.
30. White, F.M.; Majdalani, J. *Viscous Fluid Flow*; McGraw-Hill New York **2006**, *3*, 433–434.
31. Huh, D.; Kim, H.J.; Fraser, J.P.; Shea, D.E.; Khan, M.; Bahinski, A.; Hamilton, G.A.; Ingber, D.E. Microfabrication of Human Organs-on-Chips. *Nat. Protoc.* **2013**, *8*, 2135–2157. DOI:10.1038/nprot.2013.137.
32. Stucki, A.O.; Stucki, J.D.; Hall, S.R.R.; Felder, M.; Mermoud, Y.; Schmid, R.A.; Geiser, T.; Guenat, O.T. A Lung-on-a-Chip Array with an Integrated Bio-Inspired Respiration Mechanism. *Lab Chip* **2015**, *15*, 1302–1310. DOI:10.1039/C4LC01252F.
33. Ochs, C.J.; Kasuya, J.; Pavesi, A.; Kamm, R.D. Oxygen Levels in Thermoplastic Microfluidic Devices during Cell Culture. *Lab Chip* **2014**, *14*, 459–462. DOI: 10.1039/c3lc51160j.
34. Augusto, L.L.X.; Gonçalves, J.A.S.; Lopes, G.C. CFD Evaluation of the Influence of Physical Mechanisms, Particle Size, and Breathing Condition on the Deposition of Particulates in a Triple Bifurcation Airway. *Water, Air, Soil Pollut.* **2016**, *227*, 56. DOI:10.1007/s11270-016-2753-y.
35. Friedlander, S.K.; Smoke, D. *Haze: Fundamentals of Aerosol Dynamics*, **2000**.
36. Knotter, D.M.; Wali, F. Developments in Surface Contamination and Cleaning. *Particle Deposition, Control and Removal 1st edn*, **2010**, 81–120. DOI: 10.1016/B978-1-4377-7830-4.10003-9 2010.
37. Hayter, A.J. *Probability and Statistics for Engineers and Scientists*; Cengage Learning, **2012**. ISBN 1133712762.
38. Frost, T.S.; Jiang, L.; Zohar, Y. Pharmacokinetic Analysis of Epithelial/Endothelial Cell Barriers in Microfluidic Bilayer Devices with an Air–Liquid Interface. *Micromachines* **2020**, *11*, 536. DOI: 10.3390/mi11050536.