

Disclaimer/Publisher's Note: The statements, opinions, and data contained in all publications are solely those of the individual author(s) and contributor(s) and not of MDPI and/or the editor(s). MDPI and/or the editor(s) disclaim responsibility for any injury to people or property resulting from any ideas, methods, instructions, or products referred to in the content.

Article

Effect of Aging of Orthodontic Aligners in Different Storage Media on Force and Torque Generation: An in vitro Study

Tarek M. Elshazly ^a^{1†}, Diva Nang ^a[†], Bijan Golkhani ^a, Hanaa Elattar ^{b, c} and Christoph Bouraue ^a

^a Oral Technology, Dental School, University Hospital Bonn, Bonn, Germany

^b Orthodontic Department, Faculty of Dentistry, Umm Al-Qura University, Makkah, Saudi Arabia

^c Orthodontic Department, Faculty of Dentistry, Suez Canal University, Ismailia, Egypt

† These authors have contributed equally to this work and share the first authorship

Abstract

The aim of this study is to study the effect of aging in different media (deionized water and artificial saliva) on the force/torque generation by thermoplastic orthodontic aligners. Ten thermoformed aligners made of Essix ACE® thermoplastic sheets were aged in deionized water and in artificial saliva over two weeks at 37 °C, five in each medium. The force/torque generated on upper second premolar (Tooth 25) of a resin model was measured at day 0 (before aging), 2, 4, 6, 10, and 14, using a biomechanical test set-up. The results showed that the thermocycling of aligners has no significant impact on their force/torque decay. No significant differences were also found in force/torque between the aligners stored in deionized water nor artificial saliva. The vertical extrusion-intrusion forces were measured in the range of 1.4 to 4.6 N, the horizontal oro-vestibular forces were 1.3 to 2.5 N, while the torques on mesio-distal rotation were 5.4 to 41.7 Nmm. It could be concluded that the influence of saliva on the mechanical properties can be classified as insignificant, and no significant difference between artificial aging in deionized water or artificial saliva was observed.

¹ Correspondence to:

Dr.med.dent. Tarek Elshazly

Oral Technology, University Hospital Bonn, Bonn, Germany

Welschnonnenstr. 17, 53111 Bonn, Germany

Phone: +4917634452457 | +201020700323

Fax: +49 228 2872 2588

E-mail: tarek.m.elshazly@gmail.com

ORCID: 0000-0002-3219-9048

Keywords: Biomechanics; Orthodontic force; Torque; Tooth Movement; Removable Thermoplastic Appliance; Aging; Aligners

Research Highlights

- Aging effect of saliva on mechanical properties of aligners is insignificant.
- In artificial aging, artificial saliva or deionized water have similar effect.
- The experimental studies of aligners have limitations.
- Force generation by aligner is direction dependent.

1. Introduction

In the last two decades, orthodontic aligners have become very popular among patients due to their transparent, aesthetic appearance and high wearing comfort and are preferred to fixed orthodontic braces [1–3]. Initially, the fabrication of aligners was done manually, which took a lot of effort and time. Thanks to CAD/CAM and intraoral scanner technology, the workflow has become much easier and faster [4]. The mechanical performance of orthodontic aligners is still vague [5–7]. It is assumed that the returning forces of the aligners on the target tooth are generated by two mechanisms: initially by the local elastic deformation of the aligner body in the contact area with the misaligned target tooth and then comes the elastic deformation of the entire aligner, since the entire aligner body is lifted in the area of the misaligned target tooth while it is fixed to the other teeth by friction [8, 9]. Elshazly et al. [6], based on their finite element study, postulated that the deformation of the aligner is a combination of stretching (direct proportional with deflection) and bending (direct proportional to the third power of the thickness).

The materials used have a strong effect on the performance of orthodontic aligners [5, 6]. Ideally, the orthodontic material should deliver a continuous light force throughout the treatment period [10, 11]. In addition, the material should return to its original shape after removal from the oral cavity. For this purpose, the material should have sufficient stiffness to apply the required light force and a sufficiently high elastic limit to avoid permanent deformation [12]. However, the commonly used aligner sheets are made of viscoelastic thermoplastic polymers [4, 7, 13]. Viscoelastic materials show phenomena of creep and stress relaxation, which means that their mechanical behavior differs significantly over time under different loading conditions [12, 14].

The aligners are supplied to patients in the form of a set of plastic splints. Patients are instructed to wear each aligner for at least 22 hours per day for 14 days and then replace it with its successor [15]. This means that the aligners should only be removed when eating or brushing teeth [4–7]. During function in mouth, the aligners are subjected to thermal and mechanical alternating loads. In some experimental studies [16–20] it was determined that both mechanical pre-loading and thermocycling significantly affect the mechanical properties of aligner materials, resulting in an increase in Vickers hardness [16–18], a decrease in the modulus of elasticity, as well as a reduction in strength [19, 20]. Other studies [14, 15, 21] reported that aligner materials show a significant force-drop at the first few hours of use. Drake et al. [22], in an in-vivo study, reported that the tooth movement by aligners occurs mainly within the first week of use, thus the intraoral aging of the aligner materials has insignificant effect on the magnitude of tooth movement.

Therefore, clinical aspects should be considered when investigating the material behavior of orthodontic aligners, and either an in vivo study should be conducted or the clinical situation should be mimicked in vitro [23]. In the literature, different media have been experimentally used to study aging of aligner materials. To our

knowledge, no study has investigated whether the type of aging medium used can affect the mechanical behavior of the material. Therefore, the aim of the present experiment was to investigate the influence of different aging media (deionized water and artificial saliva) on the force/torque generation by thermoformed orthodontic aligners made of thermoplastic sheets.

2. Materials and Methods

Ten thermoplastic sheets of Essix ACE® (Dentsply Sirona, Bensheim, Germany) were utilized. The aligners were fabricated by thermoforming process (according to the manufacturer's instructions), using a standard thermoforming device (Ministar S®, Scheu-Dental, Iserlohn, Germany), over an aligned maxillary arch model made of a fast-cold-curing resin (Technovit 4004, Kulzer, Hanau, Germany). The thermoformed aligners were then trimmed in a scalloped form following the gingival margin (Figure 1). As all aligners were made identically on the same model and by a solo well-trained technician, the effect of the aligner geometry on the measurements was negligible.

To study the effect of storage medium at mouth temperature (37 °C), five aligners were stored in a container with deionized water (Ampuwa, Fresenius Kabi, Bad Homburg, Germany) and another five in a container with modified artificial saliva. The composition of the artificial saliva was prepared according to Fusayama by Geis-Gerstorfer and Weber [24] (Table 1).

Force/torque measurements were carried out using the Orthodontic Measurement and Simulation System (OMSS) (Figure 1) [7, 25–27] before starting storage (Day 0) and on the 2nd, 4th, 6th, 10th, and 14th day (± 2 hours) after starting storage. The OMSS is able to simulate three-dimensional tooth movements and measure force/deflection or torque/rotation ratios. For OMSS measurement, an additional resin replica model was created, in which the upper left second premolar (Tooth 25) was separated and its neighboring teeth were slightly ground proximally to ensure that the tooth was inserted without resistance. Tooth 25 was then connected to one of the two force/torque sensor of the OMSS, while the resin model was fixed to the second sensor (Figure 1). The occlusal plane of the resin model was adjusted parallel to the sensor Y- and Z-axes.

The tooth was adjusted in the dental arch to be in its aligned neutral position, to ensure that no forces and/or torques were delivered by the aligner to the tooth in the starting position.

The tooth was moved by ± 0.2 mm in 0.01 mm increments in the X (intrusion/extrusion) and the Z (oro-vestibular translation) directions, and by $\pm 2^\circ$ rotated in disto-mesial direction in 0.1° increments around the X axis (rotation around the tooth axis), where positive (+) represent extrusion, vestibular, mesial directions (Figure 1). After each measurement, the adjustment of the measurement setup was checked and corrected if necessary.

For each measurement, the aligners were stored in the container and only taken out shortly before assembly in the OMSS, and then were returned to this container immediately after the measurements were completed. The measurements of five aligners could last around one hour. For each measurement, torque/rotation and force/translation curves were recorded and processed for subsequent data analysis.

Statistical Analysis

The maximum values of force and torque were extracted for each group, and mean values and standard deviations of all values at maximum deflection were calculated. The results were presented as bar graphs to illustrate the forces and torques of the aligners in different media over aging time. The differences in the primary data were checked for significance. Since the data were normally distributed, t-tests were performed. A Bonferroni correction was carried out to take into account the multiple statistical significance tests with associated data. The difference was significant when the value was less than 0.05.

3. Results

The comparison between both storage media showed that the forces and torques transmitted by the aligners stored in distilled water and those stored in artificial saliva behaved slightly erratic over time, however, they were of a similar magnitude, and therefore no trend could be concluded nor significant differences (Figures 2-4, Table 2). The mean values of forces/torques showed no significant difference from day 0 to day 2 as well as from day 0 to day 14, except for few groups. For the sake of clarity, only significances on days 2 and 14 are presented (Table 2). During the intrusion-extrusion movement (Tx) (Figure 2), the mean values of vertical forces generated by the aligners before storage were -2.4 ± 0.9 N for intrusion and 1.5 ± 0.5 N for extrusion, and after storage minimum measured forces were -2.2 ± 0.6 N for intrusion and 1.4 ± 0.8 N for extrusion. In the oro-vestibular translation (Tz) (Figure 3), the mean values of horizontal forces generated by the aligners before storage were -1.7 ± 0.2 N for oral translation and 2.3 ± 0.2 N for vestibular translation, and after storage minimum measured forces were -1.3 ± 0.4 N for oral translation and 2.1 ± 0.2 N for vestibular translation. Also, with the disto-mesial rotation (Rx) (Figure 4), the mean values of torque generated by the aligners before storage were -41.7 ± 11.2 Nmm for distal-rotation and 14.2 ± 4.7 Nmm for mesial-rotation, and after storage minimum measured torque were -8.1 ± 4.1 Nmm for distal-rotation and 2.0 ± 2.3 Nmm for mesial-rotation.

4. Discussion

As an active orthodontic appliance, aligners should basically have the property of exerting force evenly over time [4, 7, 18]. However, aligners are exposed to various intraoral loads which may affect their mechanical properties and thus their effectiveness [23]. Mechanical stresses in the oral cavity include short-term insertion and removal of the aligner, as well as the long-term contact with teeth [12]. Other environmental conditions that may affect the mechanical properties of aligners intraorally include water absorption and temperature changes [28]. Both effects can lead to a weakening of the aligner material over time, which occurs faster at 37 °C than at room temperature [14]. Furthermore, when the polymer sheets are stored in water, the water is absorbed by diffusion, allowing the water molecules to get between the polymer chains, which facilitates their movement. With increasing temperature, the mobility of the polymer molecules also increases, leading to changes in the material [20, 29–31].

In the present work, aligners made of Essix ACE® sheets (copolyester of a polyethylene terephthalate (PET) with 0.75 mm thickness) were studied to investigate the influence of artificial aging in two different media on the generation of forces/torques. For that, aligners were aged over two weeks at mouth temperature (37 °C) in deionized water and in artificial saliva. The artificial saliva was prepared according to Fusayama by Geis-Gerstorfer and Weber [24], which is used primarily in corrosion test procedures for metallic dental materials [32]. However, since the oral flora contains excretory products and plaque deposits, the use of artificial saliva is only an approximation of the in vivo situation, and individual factors and variations in saliva composition are not taken into account [32, 33]. The current results suggest that the use of artificial saliva is not necessary in experimental studies of aging because there are no significant differences in the generation of torques/forces compared to deionized water.

To create a realistic simulation of mechanical intraoral conditions, the Orthodontic Measurement and Simulation System (OMSS) was used, which is equipped with a temperature-controlled chamber, whose temperature was set at 37 °C. With the help of its force/torque sensors and in conjunction with the three-dimensional variable positioning tables and the corresponding software, it allows the dynamic acquisition of the orthodontic tooth movement [25, 26]. However, the rigid connection and the absence of the periodontal ligament (PDL) are a limitation of this technique.

The results of the current study showed that the vertical intrusion-extrusion forces were measured in the range of (1.4 - 4.6) N, the horizontal oro-vestibular forces were (1.3 - 2.5) N, while the torques on disto-mesial rotation were (5.4 - 41.7) Nmm. Also, the generation of forces and torques is direction-dependent, referring to the different oral and vestibular morphologies of each tooth [6].

Proffit [34] recommended forces of 0.1 - 0.2 N for intrusion, and 0.35 - 0.6 N for uncontrolled tipping and rotation. The literature does not offer any clear guidelines with regard to the torque, but one could set the values mentioned in relation to the root surface in order to get an indication of the appropriate torque for the maxillary second premolar (tooth 25), targeted tooth of the current study. Torque of 30 Nmm [35] or 20 Nmm [36] referred to a molar, which has an average root surface of about 430 mm² [37]. A root surface of 220 mm² is specified for tooth 25 [37]. Accordingly, the appropriate torque for tooth 25 is around 15.8 Nmm, which is consistent with that reported by Sander et al. [38] who measured torque during rotation of premolars and canines.

The intrusive-extrusion forces in this study averaged a maximum of 4.6±0.7 N, which is up to 20 times higher than the 0.1 - 0.2 N recommended by Proffit. The reason why such recommended low forces are used for intrusion is that periodontal damage is most frequently detected with intrusions [34]. This may be of less

relevance, since the magnitude of the force generally is postulated to play a minor role in the development of side effects, as long as the tooth deflection distance is less than or equal to the width of PDL (0.1 - 0.3 mm), as this would not stop the capillary blood flow [39]. The incremental deflection commonly used in aligner therapy and the displacement used in the current experimental work are both within the width of the PDL. Additionally, with aligner therapy, there are mutual forces of the tooth and aligner, which lead to a reduction in the range of movement that actually comes into play [40]. Furthermore, *in vivo*, the targeted tooth moves away from the starting point and thus the force initially acting on the tooth is reduced [39].

Similar to the current study, three-dimensional measurement and simulation setups have been used in various studies. Elkholy et al. investigated the forces/torques of aligners on different teeth during different tooth movements [41–44]. They reported forces in palatal deflection of maxillary central incisor in the range of 4.5 - 7.2 N [41], and torques on a 10° mesial rotation at 73.6 Nmm [43], while the average torque of a mandibular canine on a 15° distal rotation was 42.5 Nmm [44]. It should be noted that the rotation in the present study was only 2°, which is one-fifth of the rotation in the study by Elkholy et al. [43]. In addition, the present aligners were artificially aged, which could also speak for the reduced force/torques in comparison. Similarly, Hahn et al. [8, 9] reported horizontal forces on an upper central incisor tilted by 0.15 mm of 2.7 N for vestibular tilting and 3.1 N for oral tilting, which are also consistent with the oro-vestibular translation values of the present study, in terms of deflection (0.2 mm), aging, and material type. Likewise, Engelke et al. [45] studied the force and torque generation of aligners on a maxillary central incisor after simulated aging. Torques were measured between 4.3 - 20.2 Nmm, similar to the current work.

Using pressure-sensitive films, Elshazly et al. [5] reported forces of 3.8 N on a 0.2 mm bodily translation of an upper central incisor of resin model by Zendura FLX aligners trimmed in scalloped design as applied in

the current study. Similarly, Barbagallo et al. [46] reported, in an in vivo study, a mean force of 5.1 N on 0.5 mm buccally tilted maxillary first premolars, exceeding Proffit's recommendations by several times. In the current study, a maximum force of 2.5 ± 0.1 N was measured for tooth 25 in vestibular translation, which is almost 50 % of the value reported by Barbagallo. However, the maximum displacement in this work was only 0.2 mm (40 % of Barbagallo), which means that the two values are in agreement.

Kwon et al. [18] carried out 3-point bending tests on thermoplastic aligner sheets. For a 0.2 mm deflection distance of Essix ACE® sheets (0.76 mm thick), the generated force was 0.5 N before and after thermocycling with no significant difference, up to six times lower than those of current study results. The reason for this difference may be the shape of the specimen, since in the present experiment the sheets were pulled over an anatomical upper jaw model, while in Kwon's study were pulled over a flat rectangular plaster model [9, 44]. However, the results of Kwon et al. showed that the thermocycling of the aligners has no significant impact on their force loss, compatible with our results [18]. On the contrary, Barbagallo et al. [46] measured in an in-vivo study the forces at the beginning of the two-week treatment and at the end. They found that the average force decreased from 5.1 N initially to -2.7 N on the last day. It could be argued that the reason for force decay on aging is not referred to water/saliva storage (as tested in the current study) but other factors. Based on our results, the effect of aging on different materials, including mechanical loading, should be considered and investigated in future studies. In particular, that the type of material has a significant effect on the force generation by the orthodontic aligner treatment [6, 47].

5. Conclusion

- The comparison between the forces/torques over 14 days of the respective material showed no significant difference, meaning that the influence of saliva on the mechanical properties of an aligner in everyday clinical practice can be classified as insignificant.
- No significant difference between the forces/torques of the aligners stored in distilled water and those stored in artificial saliva, which means that the effect of the type of used medium for aging of aligners in vitro is insignificant.
- Generation of forces and torques by aligner is direction-dependent due to tooth morphology.

Compliance with Ethics Requirements

This article does not contain any studies with human or animal subjects.

Conflicts of interest

The authors declare no conflict of interest.

Funding

This research received no external funding

Ethical Approval

Not Applicable.

Informed Consent Statement

Not Applicable.

Authors Contributions

Conceptualization: CB

Data curation and Analysis, Investigation, and Methodology: TE, DN, CB, BG

Resources: CB

Software: Supervision, Validation and Visualization: TE, CB

Writing—original draft: TE, DN

Writing—review & editing: TE, CB, HE

All authors have read and agreed to the published version of the manuscript.

References

- [1] Ojima K. and Kau C.H. A perspective in accelerated orthodontics with aligner treatment. *Seminars in Orthodontics* 2017, 23(1), 76–82. <https://doi.org/10.1053/j.sodo.2016.10.002>
- [2] Pereira D., Machado V., Botelho J., Proença L., Mendes J.J., and Delgado A.S. Comparison of Pain Perception between Clear Aligners and Fixed Appliances: A Systematic Review and Meta-Analysis. *Appl. Sci.* 2020, 10(12), 4276. <https://doi.org/10.3390/app10124276>
- [3] Didier V.F., Almeida-Pedrin R.R., Oltramari P.V.P., Fernandes T.M.F., Dos Santos L.L., and de C.F. Conti A.C. Influence of orthodontic appliance design on employment hiring preferences. *Am. J. Orthod. Dentofac. Orthop.* 2019, 156(6), 758–766. <https://doi.org/10.1016/j.ajodo.2018.12.020>
- [4] Elshazly T.M., Keilig L., Alkabani Y., Ghoneima A., Abuzayda M., Talaat S., Bourauel C.P. Primary Evaluation of Shape Recovery of Orthodontic Aligners Fabricated from Shape Memory Polymer (A Typodont Study). *Dent. J.* 2021, 9(3), 31. <https://doi.org/10.3390/dj9030031>
- [5] Elshazly T.M., Keilig L., Salvatori D., Chavanne P., Aldesoki M., Bourauel C. Effect of Trimming Line Design and Edge Extension of Orthodontic Aligners on Force Transmission: An in vitro Study. *J. Dent.* 2022, 104276. <https://doi.org/10.1016/j.jdent.2022.104276>
- [6] Elshazly T.M., Keilig L., Aldesoki M., Ghoneima A., Abuzayda M., Talaat W., Talaat S., Bourauel C.P. Computer-aided finite element model for biomechanical analysis of orthodontic aligners. *Clin. Oral Investig.* 2022. <https://doi.org/10.1007/s00784-022-04692-7>
- [7] Elshazly T.M., Keilig L., Alkabani Y., Ghoneima A., Abuzayda M., Talaat W., Talaat S., Bourauel C.P. Potential Application of 4D Technology in Fabrication of Orthodontic Aligners. *Front. Mater.* 2022, 8, 586. <https://doi.org/10.3389/fmats.2021.794536>

- [8] Hahn W., Fialka-Fricke J., Dathe H., Fricke-Zech S., Zapf A., Gruber R., Kubein-Meesenburg D., Sadat-Khonsari R. Initial forces generated by three types of thermoplastic appliances on an upper central incisor during tipping. *Eur. J. Orthod.* 2009, 31(6), 625–631. <https://doi.org/10.1093/ejo/cjp047>
- [9] Hahn W., Dathe H., Fialka-Fricke J., Fricke-Zech S., Zapf A., Kubein-Meesenburg D., Sadat-Khonsari R. Influence of thermoplastic appliance thickness on the magnitude of force delivered to a maxillary central incisor during tipping. *Am. J. Orthod. Dentofac. Orthop.* 2009, 136(1), 12.e1-12.e7. <https://doi.org/10.1016/j.ajodo.2008.12.015>
- [10] Upadhyay M., Arquib S. A. Biomechanics of clear aligners: hidden truths & first principles. *J. World Fed. Orthod.* 2021, 12-21. <https://doi.org/10.1016/j.ejwf.2021.11.002>
- [11] Upadhyay M., Nanda R. Biomechanics in orthodontics. *Esthet. Biomech. Orthod.* 2014, 152(1), 74–89.
- [12] Lombardo L., Martines E., Mazzanti V., Arreghini A., Mollica F., Siciliani G. Stress relaxation properties of four orthodontic aligner materials: a 24-hour in vitro study. *Angle Orthod.* 2016, 87(1), 11–18. <https://doi.org/10.2319/113015-813.1>
- [13] Janda R. Organische Polymere: Chemie und Physik, Teil 1. *Quintessenz Zahntechnik* 2008, 34(2), 190.
- [14] Fang D., Zhang N., Chen H., Bai Y. Dynamic stress relaxation of orthodontic thermoplastic materials in a simulated oral environment. *Dent. Mater. J.* 2013, 32(6), 946-951. <https://doi.org/10.4012/dmj.2013-131>
- [15] Vardimon A.D., Robbins D., Brosh T. In-vivo von Mises strains during Invisalign treatment. *Am. J. Orthod. Dentofac. Orthop.* 2010, 138(4), 399–409. <https://doi.org/10.1016/j.ajodo.2008.11.027>
- [16] Schuster S., Eliades G., Zinelis S., Eliades T., Bradley T.G. Structural conformation and leaching from in vitro aged and retrieved Invisalign appliances. *Am. J. Orthod. Dentofac. Orthop.* 2004, 126(6), 725–

728. <https://doi.org/10.1016/j.ajodo.2004.04.021>

- [17] Pazzini L., Cerroni L., Pasquantonio G., Pecora A., Mussi V., Rinaldi A., Mecheri B., Licoccia S., Maiolo L. Mechanical properties of ‘two generations’ of teeth aligners: Change analysis during oral permanence *Dent. Mater. J.* 2018, 37(5), 835–842. <https://doi.org/10.4012/dmj.2017-323>
- [18] Kwon J.-S., Lee Y.-K., Lim B.-S., Lim Y.-K. Force delivery properties of thermoplastic orthodontic materials. *Am. J. Orthod. Dentofac. Orthop.* 2008, 133(2), 228–234. <https://doi.org/10.1016/j.ajodo.2006.03.034>
- [19] Ihssen B.A., Willmann J.H., Nimer A., Drescher D. Effect of in vitro aging by water immersion and thermocycling on the mechanical properties of PETG aligner material. *J. Orofac. Orthop. der Kieferorthopädie* 2019, 80(6), 292–303. <https://doi.org/10.1007/s00056-019-00192-8>
- [20] Hiller D. Elastizitaet und Dimensionsstabilitaet von Druckformfolien vor und nach Temperaturwechselbelastung. 2018. <http://dx.doi.org/10.17169/refubium-688>
- [21] Lombardo L., Arreghini A., Ramina F., Huanca Ghislanzoni L.T., Siciliani G. Predictability of orthodontic movement with orthodontic aligners: a retrospective study. *Prog. Orthod.* 2017, 18(1), 1–12. <https://doi.org/10.1186/s40510-017-0190-0>
- [22] Drake C.T., McGorray S.P., Dolce C., Nair M., Wheeler T.T. Orthodontic tooth movement with clear aligners. *ISRN Dent.* 2012, Article ID 657973. doi:10.5402/2012/657973
- [23] Nang D. Veraenderung der Materialeigenschaften kieferorthopaedischer Korrekturschienen durch kuenstliche Alterung. Universitaets-und Landesbibliothek Bonn, 2022. <https://hdl.handle.net/20.500.11811/9790>
- [24] Geis-Gerstorfer J., Weber H. Der Einfluss von Kaliumrhodanid auf das Korrosionsverhalten

- edelmetallfreier Dentallegierungen. *Dtsch zahnärztl* 1985, 40, 87–91.
- [25] Bouraue C., Drescher D., Thier M. An experimental apparatus for the simulation of three-dimensional movements in orthodontics. *J. Biomed. Eng.* 1992, 14(5), 371–378. [https://doi.org/10.1016/0141-5425\(92\)90081-U](https://doi.org/10.1016/0141-5425(92)90081-U)
- [26] Drescher D., Bouraue C., Thier M. Application of the orthodontic measurement and simulation system (OMSS) in orthodontics. *Eur. J. Orthod.* 1991, 13(3), 169–178. <https://doi.org/10.1093/ejo/13.3.169>
- [27] Simon M., Keilig L., Schwarze J., Jung B.A., Bouraue C. Forces and moments generated by removable thermoplastic aligners: incisor torque, premolar derotation, and molar distalization. *Am. J. Orthod. Dentofac. Orthop.* 2014, 145(6), 728–736. <https://doi.org/10.1016/j.ajodo.2014.03.015>
- [28] Ryokawa H., Miyazaki Y., Fujishima A., Miyazaki T., Maki K. The mechanical properties of dental thermoplastic materials in a simulated intraoral environment. *Orthod. waves* 2006, 65(2), 64–72. <https://doi.org/10.1016/j.odw.2006.03.003>
- [29] Elshazly T.M., Bouraue C., Sherief D.I., El-Korashy D.I. Evaluation of Two Resin Composites Having Different Matrix Compositions. *Dent. J.* 2020, 8(3), 76. <https://doi.org/10.3390/dj8030076>
- [30] Elshazly T.M., Bouraue C., Aboushelib M.N., Sherief D.I., El-Korashy D.I. The polymerization efficiency of a bulk-fill composite based on matrix-modification technology. *Restor. Dent. Endod.* 2020, 45(3), e32. <https://doi.org/10.5395/rde.2020.45.e32>
- [31] Elshazly T.M.. Werkstoffwissenschaftliche Untersuchung eines gefüllten, matrixmodifizierten zahnärztlichen Komposit. Universitäts- und Landesbibliothek Bonn, 2021. <https://hdl.handle.net/20.500.11811/8926>
- [32] Luft S.I. Materialtechnische Untersuchungen an selbstligierenden und konventionellen Brackets.

Universitäts-und Landesbibliothek Bonn, 2008. <https://hdl.handle.net/20.500.11811/3804>

- [33] Eliades T., Bourauel C. Intraoral aging of orthodontic materials: the picture we miss and its clinical relevance. *Am. J. Orthod. Dentofac. Orthop.* 2005, 127(4), 403–412. <https://doi.org/10.1016/j.ajodo.2004.09.015>
- [34] Proffit W.R., Fields H.W., Sarver D.M., Ackerman J.L. *Contemporary Orthodontics*. St. Louis. Mosby. Inc, 2000.
- [35] Melsen B., Burstone Ch J. The transpalatal arch and the lower lingual arch. Their use as active and passive appliance. *Melsen B, Burstone Ch, Introd. to Biomech. Syllabus Univ. Aarhus*, 1990.
- [36] Wichelhaus A., Sander C., Sander F.G. Development and biomechanical investigation of a new compound palatal arch. *J. Orofac. Orthop. der Kieferorthopädie* 2004, 65(2), 104–122. <https://doi.org/10.1007/s00056-004-0214-5>
- [37] Kahl-Nieke B. *Einführung in die Kieferorthopädie: Diagnostik, Behandlungsplanung, Therapie: mit 10 Tabellen*. Deutscher Ärzteverlag, 2010.
- [38] Sander C., Sander F.M., Sander F.G. The derotation of premolars and canines with NiTi elements. *J. Orofac. Orthop. der Kieferorthopädie* 2006, 67(2), 117–126. <https://doi.org/10.1007/s00056-006-5043-2>
- [39] Erfurth-Jach T.F. Biomechanische Untersuchungen an thermoplastisch geformten Schienen 2012. <http://dx.doi.org/10.53846/goediss-1559>
- [40] Barbagallo L.J., Jones A.S., Petocz P., Darendeliler M.A. Physical properties of root cementum: part 10. Comparison of the effects of invisible removable thermoplastic appliances with light and heavy orthodontic forces on premolar cementum. A microcomputed-tomography study. *Am. J. Orthod.*

Dentofac. Orthop. 2008, 133(2), 218–227.

- [41] Elkhol F., Panchaphongsaphak T., Kilic F., Schmidt F., Lapatki B.G. Forces and moments delivered by PET-G aligners to an upper central incisor for labial and palatal translation. *J. Orofac. Orthop.* 2015, 76, 460–475. <https://doi.org/10.1007/s00056-015-0307-3>.
- [42] Elkhol F., Schmidt F., Jäger R., Lapatki B.G. Forces and moments delivered by novel, thinner PET-G aligners during labiopalatal bodily movement of a maxillary central incisor: An in vitro study. *Angle Orthod.* 2016, 86(6), 883–890. <https://doi.org/10.2319/011316-37R.1>
- [43] Elkhol F., Mikhail B., Schmidt F., Lapatki B.G. Mechanical load exerted by PET-G aligners during mesial and distal derotation of a mandibular canine. *J. Orofac. Orthop.* 2017, 78, 361–370. <https://doi.org/10.1007/s00056-017-0090-4>
- [44] Elkhol F., Schmidt F., Jäger R., Lapatki B.G. Forces and moments applied during derotation of a maxillary central incisor with thinner aligners: an in-vitro study. *Am. J. Orthod. Dentofac. Orthop.* 2017, 151(2), 407–415. <https://doi.org/10.1016/j.ajodo.2016.08.020>
- [45] Engelke B. Kraft-und Drehmomentabgabe thermoplastisch geformter Schienen bei Frontzahnderotation vor und nach Alterungssimulation. 2010. <http://dx.doi.org/10.53846/goediss-889>
- [46] Barbagallo L.J., Shen G., Jones A.S., Swain M.V., Petocz P., Darendeliler M.A. A novel pressure film approach for determining the force imparted by clear removable thermoplastic appliances. *Ann. Biomed. Eng.* 2008, 36(2), 335–341. <https://doi.org/10.1007/s10439-007-9424-5>
- [47] Elshazly T., Salvatori D., Bourauel C., Elattar H., Alkabani Y. Effect of Thickness and Material Type of Orthodontic Aligners on Force Transmission: An in Vitro Study Using Pressure-Sensitive Films. Available at SSRN 4270102.

Legends:**Tables:**

Table 1: Composition of artificial saliva according to Geis-Gerstorfer and Weber [24]. 23

Table 2: Mean of maximum forces and torques on tooth 25 by aligners made from Essix ACE® sheets before and after aging (2 and 14 days) in deionized water compared to storage in artificial saliva..... 24

Figures:

Figure 1: Resin model with aligner fitted in the orthodontic measurement and simulation system (OMSS): The tooth to be moved (Tooth 25) was adjusted in the aligned position in the aligner. Simulation of three tooth movements: intrusion/extrusion by 0.2 mm (X axes) (upper), oro-vestibular translation by 0.2 mm (Z axes), and 2° rotation around the tooth axis in disto-mesial direction (around X axes) (lower)..... 26

Figure 2: Mean of maximum intrusive/extrusive forces on tooth 25 generated by aligners made from Essix ACE® sheets after aging in deionized water and in artificial saliva at 37 °C..... 27

Figure 3: Mean of maximum oro-vestibular forces on tooth 25 generated by aligners made from Essix ACE® sheets after aging in deionized water and in artificial saliva at 37 °C..... 28

Figure 4: Mean of maximum torque upon rotation (disto-mesial rotation) around tooth 25 axes generated by aligners made from Essix ACE® sheets after aging in deionized water and in artificial saliva at 37 °C. 29

Table 1: Composition of artificial saliva according to Geis-Gerstorfer and Weber [24].

| Component | Molecular Formula | Concentration (mg/L) |
|-------------------------------------|--|--------------------------------------|
| Sodium Chloride | NaCl | 400 |
| Potassium Chloride | KCl | 400 |
| Calcium Chloride Dihydrate | CaCl ₂ .2H ₂ O | 795 |
| Sodium Hydrogen Phosphate 1-Hydrate | NaH ₂ PO ₄ .H ₂ O | 690 |
| Potassium Rhodanide | KSCN | 300 |
| Sodium Sulfide | Na ₂ S.9H ₂ O | 1.67 [normal with 5H ₂ O] |
| Urea | CH ₄ N ₂ O | 1000 |

Table 2: Mean of maximum forces and torques on tooth 25 by aligners made from Essix ACE® sheets before and after aging (2 and 14 days) in deionized water compared to storage in artificial saliva.

| | | Intrusion Force (N) | p-value | Extrusion Force (N) | p-value |
|----------------|---------------------------|-----------------------------|----------|-----------------------------|--------------------------|
| Aging | Deionized Water | Artificial Saliva | | Deionized Water | Artificial Saliva |
| 0 day | -2.4±0.9 ^A | -2.4±0.9 ^B | - | 1.5±0.5 ^A | 1.5±0.5 ^A |
| 2 days | -3.1±0.6 ^{Ab} | -4.6±0.7 ^{AA} | *p<0.05 | 1.5±0.6 ^{AA} | 1.9±0.6 ^{AA} |
| 14 days | -3.8±5.1 ^{AA} | -3.6±1.9 ^{ABA} | 0.899 | 4.6±6.3 ^{AA} | 1.6±0.6 ^{AA} |
| p-value | 0.899 | * p<0.05 | | 0.899 | 0.899 |
| | | Oral Force (N) | p-value | Vestibular Force (N) | p-value |
| Aging | Deionized Water | Artificial Saliva | | Deionized Water | Artificial Saliva |
| 0 day | -1.7±0.2 ^A | -1.7±0.2 ^A | - | 2.3±0.2 ^A | 2.3±0.2 ^A |
| 2 days | -1.5±0.0 ^{Ab} | -1.7±0.1 ^{AA} | *p<0.05 | 2.2±0.0 ^{Ab} | 2.3±0.1 ^{ABA} |
| 14 days | -1.3±0.4 ^{Ab} | -2.0±0.2 ^{AA} | *p<0.05 | 2.2±0.2 ^{AA} | 2.1±0.2 ^{Ba} |
| p-value | 0.899 | 0.899 | | 0.899 | * p<0.05 |
| | | Distalrotation Torque (Nmm) | p-value | Mesialrotation Torque (Nmm) | p-value |
| Aging | Deionized Water | Artificial Saliva | | Deionized Water | Artificial Saliva |
| 0 day | -41.7 ± 11.2 ^A | -41.7 ± 11.2 ^A | - | 14.2 ± 4.7 ^A | 14.2 ± 4.7 ^A |
| 2 days | -20.4 ± 4.0 ^{Ba} | -20.3 ± 4.6 ^{Ba} | 0.899 | 6.3 ± 2.7 ^{Bb} | 15.5 ± 4.8 ^{AA} |
| 14 days | -8.1 ± 4.1 ^{Bb} | -15.0 ± 5.1 ^{Ba} | * p<0.05 | 16.1 ± 6.9 ^{AA} | 14.4 ± 4.9 ^{AA} |
| p-value | * p<0.05 | *p<0.05 | | * p<0.05 | 0.899 |

Different upper and lowercase superscript letters indicate a statistically significant difference within the same vertical column and horizontal row respectively, *significant ($p<0.05$)

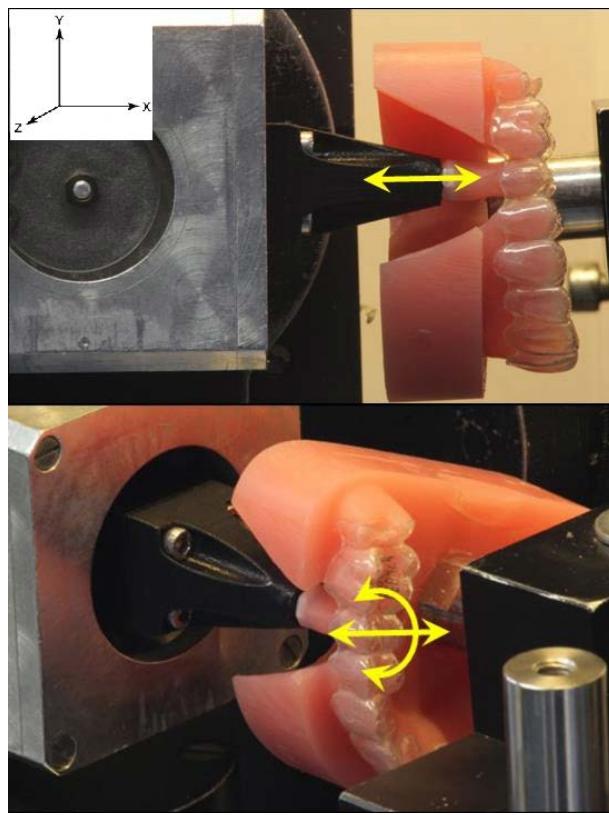


Figure 1: Resin model with aligner fitted in the orthodontic measurement and simulation system (OMSS): The tooth to be moved (Tooth 25) was adjusted in the aligned position in the aligner. Simulation of three tooth movements: intrusion/extrusion by 0.2 mm (X axes) (upper), oro-vestibular translation by 0.2 mm (Z axes), and 2° rotation around the tooth axis in disto-mesial direction (around X axes) (lower).

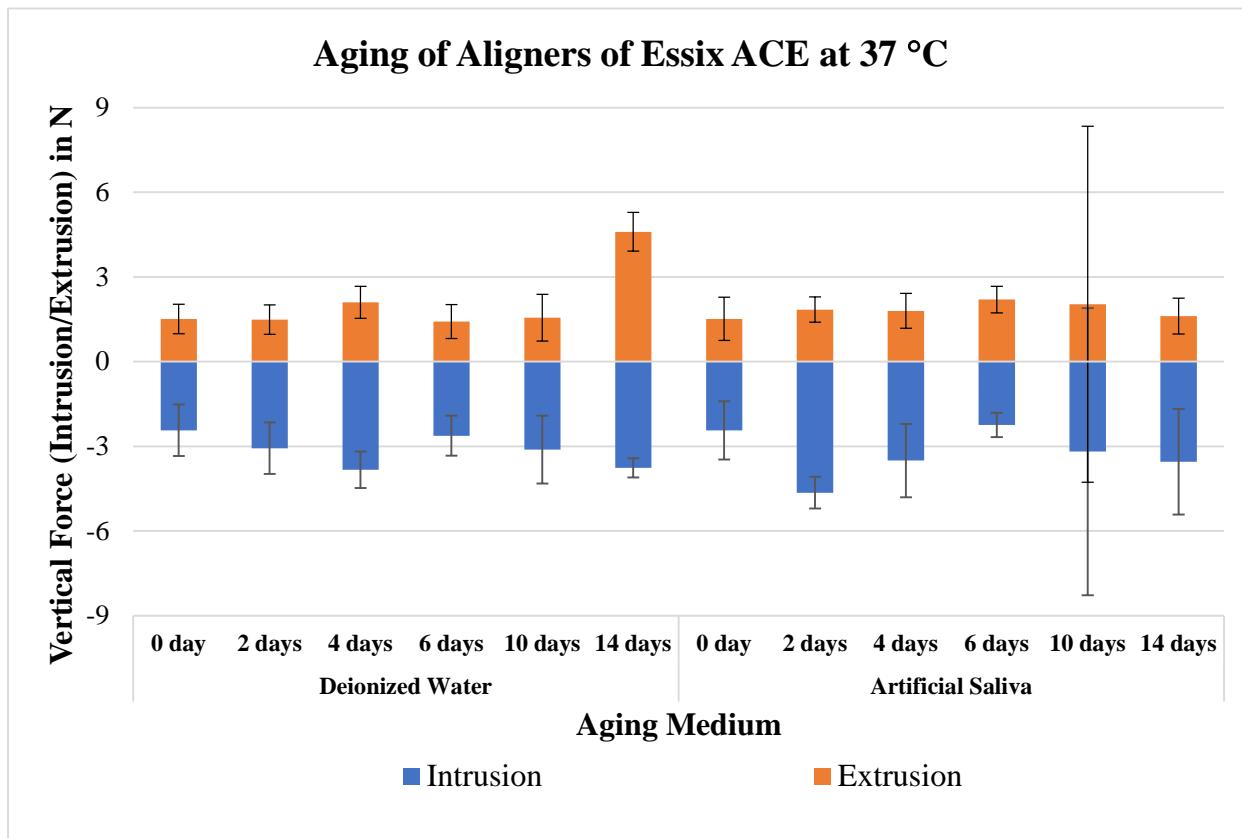


Figure 2: Mean of maximum intrusive/extrusive forces on tooth 25 generated by aligners made from Essix ACE® sheets after aging in deionized water and in artificial saliva at 37 °C.

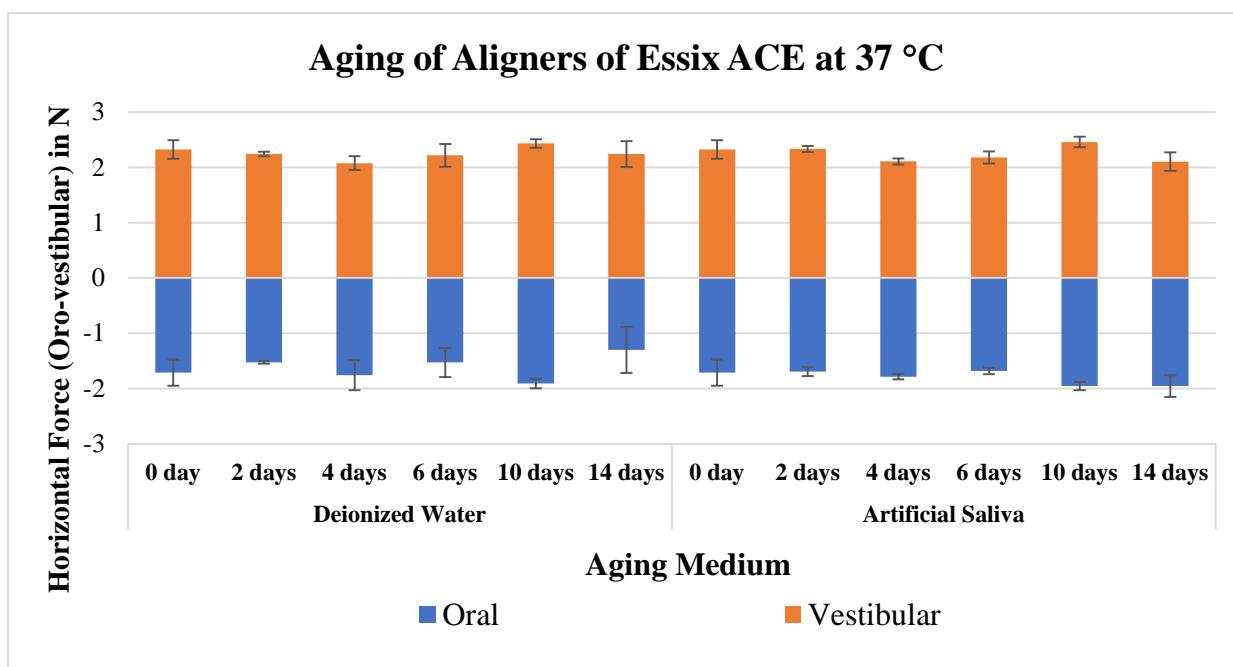


Figure 3: Mean of maximum oro-vestibular forces on tooth 25 generated by aligners made from Essix ACE® sheets after aging in deionized water and in artificial saliva at 37 °C.

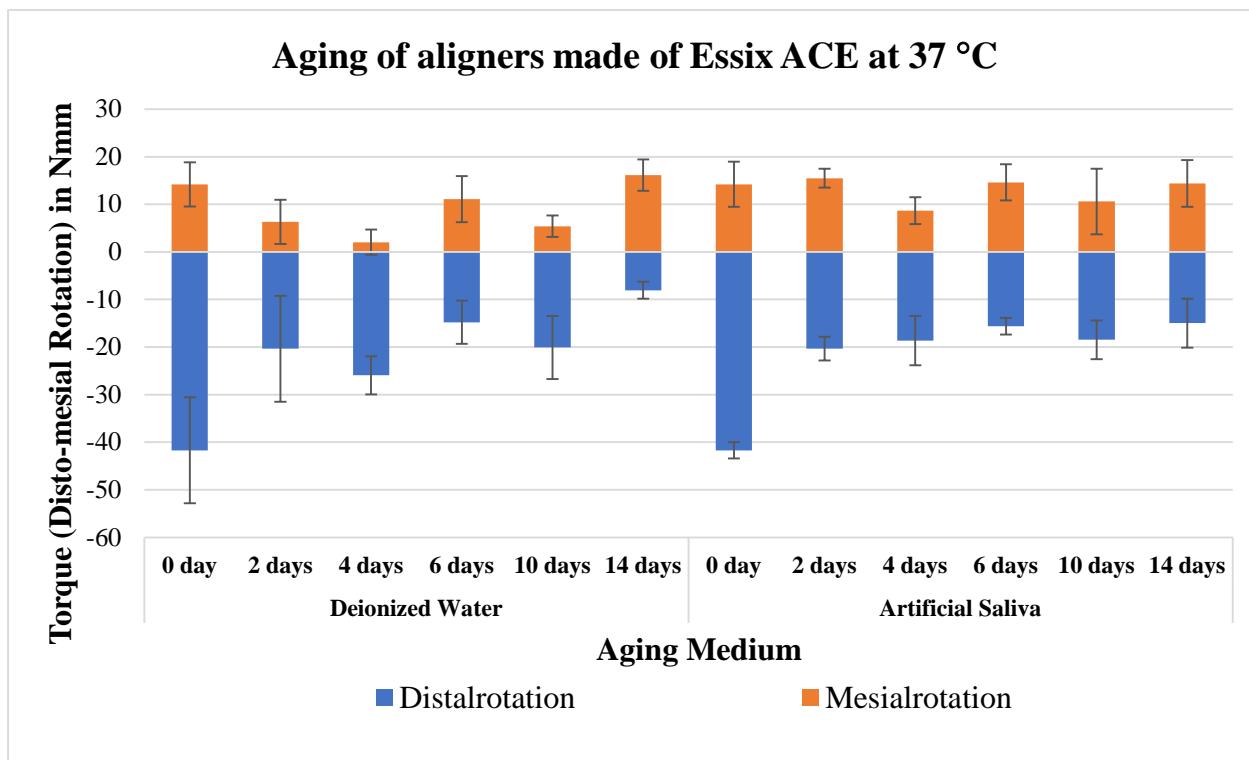


Figure 4: Mean of maximum torque upon rotation (disto-mesial rotation) around tooth 25 axes generated by aligners made from Essix ACE® sheets after aging in deionized water and in artificial saliva at 37 °C.